


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU010923\
Data File : VU052634.D
Acq On : 09 Jan 2023 09:37
Operator : JC/MD
Sample : BFB152
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB152

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010623WMA.M
Title : VOC Analysis
Last Update : Mon Jan 09 20:59:53 2023

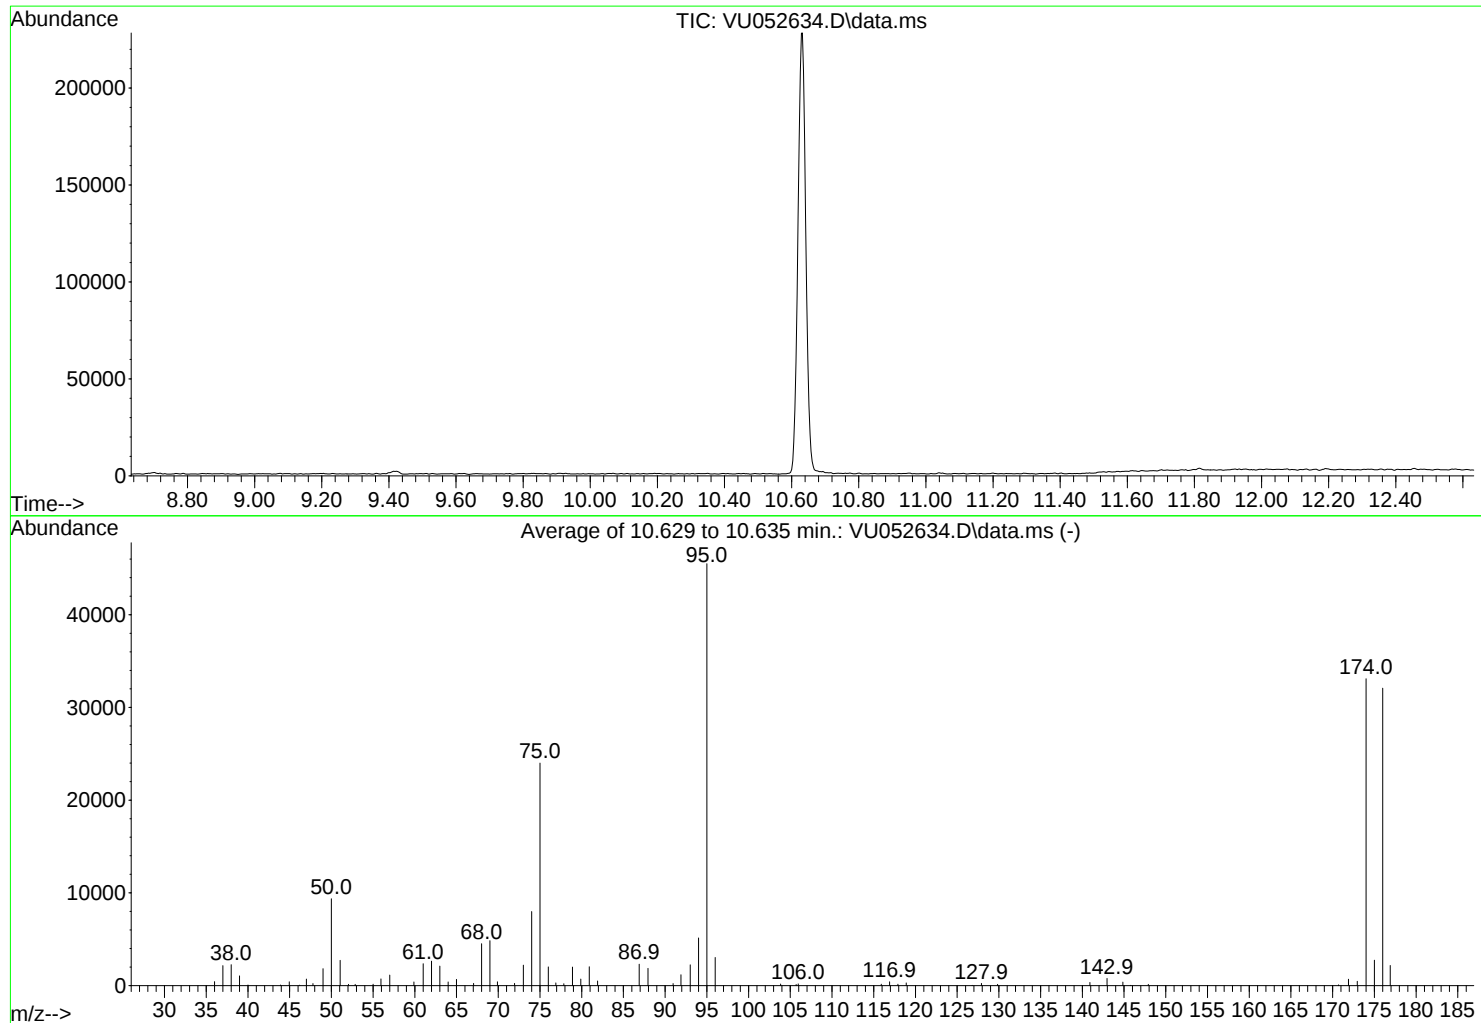

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	9363	PASS
75	95	30	80	52.8	24008	PASS
95	95	100	100	100.0	45499	PASS
96	95	5	9	6.7	3028	PASS
173	174	0.00	2	1.4	465	PASS
174	95	50	120	72.8	33101	PASS
175	174	5	9	8.3	2740	PASS
176	174	95	101	96.9	32085	PASS
177	176	5	9	6.8	2173	PASS

m/z	Abundance
39.90	155.0
43.90	861.0
126.80	256.0

Instrument :
MSVOA_U
ClientSampleId :
BFB152

m/z	Abundance
35.90	431.0
37.00	2369.0
38.00	2240.0
39.00	1067.0
39.80	227.0
43.90	968.0
45.00	438.0
47.00	640.0
47.80	216.0
49.00	1946.0
50.00	9795.0
51.10	2900.0
52.00	130.0
52.80	125.0
55.00	141.0
55.90	713.0
57.00	1148.0
59.90	427.0
61.00	2500.0
62.00	2584.0
63.00	2136.0
64.00	437.0
65.00	676.0
67.00	245.0
68.00	4719.0
69.00	5079.0
69.90	422.0
71.90	246.0
73.00	2261.0
74.00	8795.0
75.00	25040.0
76.00	2183.0
76.90	352.0
78.00	182.0
78.90	2029.0
79.90	756.0
80.90	2138.0
81.90	470.0
86.90	2348.0
87.90	1987.0
91.00	185.0
91.90	1214.0
93.00	2455.0
94.00	5322.0
95.00	46720.0
96.00	3310.0
103.90	165.0
105.70	158.0
106.00	166.0
115.90	133.0
116.90	356.0
117.80	125.0
118.90	282.0
126.80	302.0
128.00	247.0
129.80	148.0
140.90	330.0
142.90	761.0
144.80	408.0
147.90	132.0
171.90	647.0
173.00	512.0
174.00	33200.0
175.00	2768.0
176.00	32440.0
176.90	2262.0

Instrument :
MSVOA_U
ClientSampleId :
BFB152

m/z	Abundance
36.00	413.0
37.00	2189.0
38.00	2383.0
39.00	1083.0
39.80	206.0
43.90	914.0
44.90	398.0
47.00	723.0
47.80	213.0
49.00	1883.0
50.00	9708.0
51.10	2841.0
52.10	146.0
52.90	135.0
55.00	164.0
56.00	741.0
57.00	1133.0
59.90	385.0
61.00	2447.0
62.00	2756.0
63.00	2165.0
64.00	402.0
65.00	670.0
67.10	249.0
68.00	4594.0
69.00	4988.0
69.90	404.0
72.00	240.0
73.00	2264.0
74.00	8312.0
75.00	24648.0
76.00	2055.0
76.90	290.0
77.80	209.0
78.90	2059.0
79.90	751.0
80.90	2077.0
81.90	508.0
86.90	2418.0
87.90	1855.0
91.00	220.0
91.90	1157.0
93.00	2284.0
94.00	5293.0
95.00	46904.0
96.00	3103.0
103.90	173.0
105.70	164.0
105.90	164.0
115.90	159.0
116.90	403.0
117.90	132.0
118.90	292.0
126.80	284.0
127.90	251.0
129.80	137.0
140.90	348.0
142.90	765.0
144.90	404.0
147.90	138.0
170.70	112.0
171.90	715.0
172.90	470.0
174.00	34112.0
175.00	2851.0
176.00	33064.0
176.90	2265.0

Instrument :
MSVOA_U
ClientSampleId :
BFB152

m/z	Abundance
36.10	419.0
37.00	1869.0
38.00	2124.0
39.00	965.0
40.00	166.0
44.00	873.0
44.90	389.0
46.20	108.0
47.00	723.0
47.80	233.0
49.00	1638.0
50.00	8585.0
51.00	2436.0
52.10	127.0
52.90	129.0
55.00	142.0
56.00	680.0
57.00	1120.0
59.90	369.0
61.00	2141.0
62.00	2577.0
63.00	1976.0
64.00	336.0
65.00	635.0
67.10	183.0
68.00	4229.0
69.00	4472.0
69.90	367.0
72.00	227.0
73.00	2059.0
74.00	6857.0
75.00	22336.0
76.00	1773.0
76.90	202.0
77.80	231.0
78.90	1882.0
79.90	619.0
80.90	1850.0
81.90	516.0
86.90	2141.0
88.00	1705.0
90.90	263.0
91.90	1125.0
93.00	1970.0
94.00	4800.0
95.00	42872.0
96.00	2671.0
103.80	150.0
105.90	191.0
115.90	165.0
116.90	442.0
118.00	162.0
118.90	296.0
126.80	254.0
127.80	200.0
129.90	119.0
140.90	332.0
143.00	772.0
144.90	327.0
145.80	103.0
147.90	115.0
170.70	115.0
171.90	690.0
172.90	412.0
174.00	31992.0
175.00	2602.0
176.00	30752.0
176.90	1991.0

Instrument :
MSVOA_U
ClientSampleId :
BFB152