
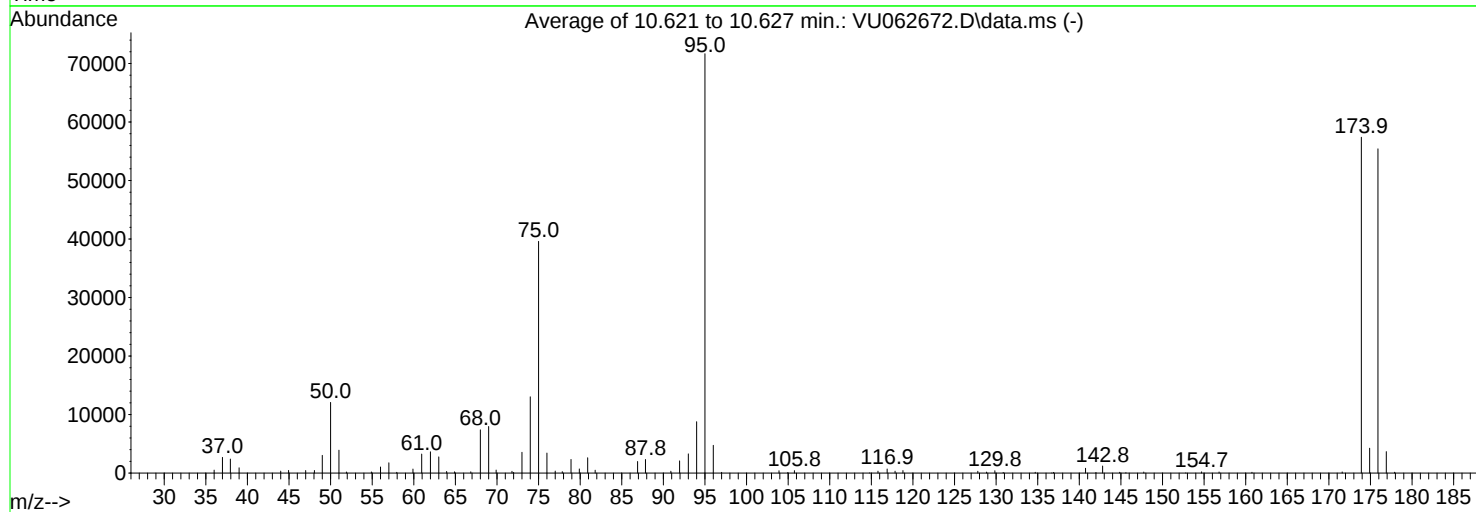


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011025\
Data File : VU062672.D
Acq On : 10 Jan 2025 09:09
Operator : MD/SY
Sample : BFB058
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB058

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jan 10 22:42:03 2025

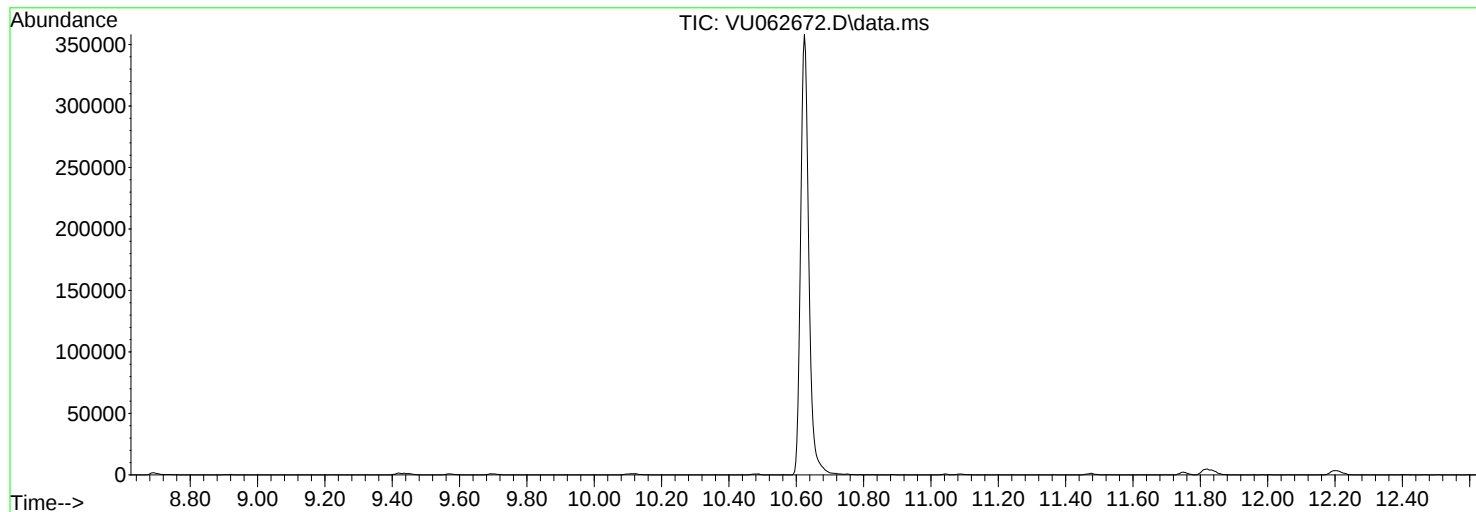

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	12082	PASS
75	95	30	80	55.2	39597	PASS
95	95	100	100	100.0	71669	PASS
96	95	5	9	6.6	4743	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.1	57392	PASS
175	174	5	9	7.4	4248	PASS
176	174	95	101	96.6	55419	PASS
177	176	5	9	6.6	3669	PASS

m/z

Abundance

Instrument :

MSVOA_U

ClientSampleId :

BFB058

m/z	Abundance
36.00	548.0
37.00	2602.0
38.00	2443.0
39.00	908.0
44.00	329.0
45.00	436.0
47.00	383.0
48.10	428.0
49.00	3098.0
50.00	12114.0
51.00	3979.0
51.90	215.0
54.90	219.0
56.00	996.0
57.00	1782.0
58.00	117.0
59.90	665.0
60.90	3075.0
62.00	3575.0
63.00	2765.0
64.00	313.0
64.90	299.0
66.90	217.0
68.00	7359.0
69.00	7837.0
69.90	505.0
71.80	485.0
73.00	3448.0
74.00	12798.0
75.00	39440.0
76.00	3302.0
77.00	365.0
77.80	258.0
78.90	2269.0
79.90	704.0
80.90	2584.0
81.80	515.0
86.90	2058.0
87.90	2302.0
90.90	338.0
92.00	2116.0
93.00	3106.0
94.00	8694.0
95.00	70680.0
96.00	4734.0
97.00	139.0
103.90	396.0
104.90	128.0
105.70	455.0
115.80	305.0
116.90	668.0
117.80	293.0
118.80	374.0
127.80	324.0
128.90	175.0
129.90	411.0
130.90	123.0
134.70	147.0
136.70	117.0
140.70	847.0
142.80	1136.0
144.80	112.0
147.80	182.0
152.80	102.0
154.70	232.0
156.80	220.0
160.70	128.0
171.60	178.0
173.90	55328.0
174.90	4043.0
175.90	53808.0
176.90	3728.0
177.90	151.0

Instrument :
MSVOA_U
ClientSampleId :
BFB058

m/z	Abundance
36.00	519.0
37.00	2749.0
38.00	2453.0
39.00	921.0
44.00	336.0
45.00	467.0
47.00	450.0
48.10	468.0
49.00	3100.0
50.00	12467.0
51.00	4074.0
51.90	211.0
54.90	197.0
56.00	1087.0
57.00	1804.0
57.90	128.0
59.90	682.0
61.00	3308.0
62.00	3762.0
63.00	2859.0
63.90	283.0
64.90	225.0
66.80	230.0
68.00	7672.0
69.00	8222.0
69.90	533.0
71.80	433.0
73.00	3664.0
74.00	13337.0
75.00	40800.0
76.00	3554.0
77.00	351.0
77.90	256.0
78.90	2425.0
79.90	727.0
80.90	2671.0
81.80	514.0
86.90	2052.0
87.90	2443.0
90.90	338.0
92.00	2092.0
93.00	3406.0
94.00	8941.0
95.00	74000.0
96.00	4827.0
97.00	119.0
103.90	404.0
105.00	127.0
105.70	410.0
115.80	343.0
116.90	759.0
117.80	341.0
118.80	470.0
127.80	333.0
128.90	191.0
129.80	429.0
130.80	117.0
134.70	141.0
136.90	159.0
140.70	854.0
142.00	137.0
142.80	1236.0
144.80	144.0
145.60	117.0
147.70	203.0
154.70	220.0
156.80	209.0
160.70	153.0
171.60	213.0
173.90	58992.0
174.90	4310.0
175.90	56912.0
176.90	3796.0
177.90	167.0

Instrument :
MSVOA_U
ClientSampleId :
BFB058

m/z	Abundance
36.00	470.0
37.00	2698.0
37.90	2293.0
39.00	875.0
44.00	346.0
44.90	456.0
47.00	472.0
48.00	424.0
49.00	2884.0
50.00	11665.0
51.00	3691.0
51.90	158.0
54.90	185.0
56.00	1059.0
57.00	1692.0
57.90	156.0
59.90	716.0
61.00	3366.0
62.00	3566.0
63.00	2688.0
64.00	249.0
64.80	145.0
66.80	235.0
68.00	7136.0
69.00	7825.0
69.90	511.0
72.00	345.0
73.00	3550.0
74.00	12975.0
75.00	38552.0
76.00	3423.0
77.00	331.0
77.90	219.0
78.90	2301.0
79.90	684.0
80.90	2601.0
81.80	449.0
86.90	1818.0
87.80	2221.0
90.90	300.0
91.90	2034.0
93.00	3335.0
94.00	8692.0
95.00	70328.0
96.00	4668.0
97.00	107.0
103.90	408.0
105.80	389.0
114.80	118.0
115.80	345.0
116.90	675.0
117.90	367.0
118.80	455.0
127.80	294.0
128.80	170.0
129.90	380.0
130.80	111.0
134.70	121.0
136.90	176.0
140.80	762.0
142.00	150.0
142.80	1248.0
144.90	153.0
145.60	117.0
147.80	176.0
154.70	192.0
156.80	153.0
160.80	127.0
171.60	218.0
173.90	57856.0
174.90	4391.0
175.90	55536.0
176.90	3484.0
177.90	133.0

Instrument :
MSVOA_U
ClientSampleId :
BFB058