

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011222\
 Data File : VU046738.D
 Acq On : 12 Jan 2022 13:28
 Operator : SY/MD
 Sample : N1101-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXW4

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/13/2022
 Supervised By :Mahesh Dadoda 01/13/2022

Quant Time: Jan 12 13:44:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jan 10 00:25:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.272	114	77339	5.000	ug/L	0.02
28) Chlorobenzene-d5	9.423	117	75636	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	45642	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	18647	3.061	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	61.200%
7) Chloroethane-d5	1.925	69	18369	3.829	ug/L	0.01
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.600%
11) 1,1-Dichloroethene-d2	2.575	65	8424	3.279	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.600%
20) 2-Butanone-d5	4.774	46	71512m	40.471	ug/L	0.12
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.940%
24) Chloroform-d	5.099	84	46197	4.139	ug/L	0.04
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.800%
26) 1,2-Dichloroethane-d4	5.735	65	27973	4.384	ug/L	0.03
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.600%
32) Benzene-d6	5.755	84	85653	4.062	ug/L	0.03
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.200%
36) 1,2-Dichloropropane-d6	6.710	67	28057	4.428	ug/L	0.02
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.600%
41) Toluene-d8	7.909	98	74041	3.869	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.400%
43) trans-1,3-Dichloroprop...	8.192	79	12257	4.183	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.600%
46) 2-Hexanone-d5	8.655	63	78448	45.599	ug/L	0.02
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.200%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	31327	4.818	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.400%
66) 1,2-Dichlorobenzene-d4	12.195	152	34310	4.081	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	81.600%
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.588	96	5116	0.752	ug/L	# 46
19) 1,1-Dichloroethane	3.874	63	2364	0.177	ug/L	100
22) cis-1,2-Dichloroethene	4.690	96	19858	2.503	ug/L	99
33) Benzene	5.800	78	23435	0.780	ug/L	100
34) Trichloroethene	6.562	95	203640	25.705	ug/L	97
42) Toluene	7.980	91	32903	1.067	ug/L	99
47) Tetrachloroethene	8.562	164	243614	43.457	ug/L	94
52) Ethylbenzene	9.575	91	4892	0.153	ug/L	99
53) m,p-Xylene	9.697	106	1772	0.145	ug/L	80
55) Styrene	10.118	104	1135	0.056	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011222\
Data File : VU046738.D
Acq On : 12 Jan 2022 13:28
Operator : SY/MD
Sample : N1101-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXW4

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/13/2022
Supervised By :Mahesh Dadoda 01/13/2022

Quant Time: Jan 12 13:44:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jan 10 00:25:50 2022
Response via : Initial Calibration

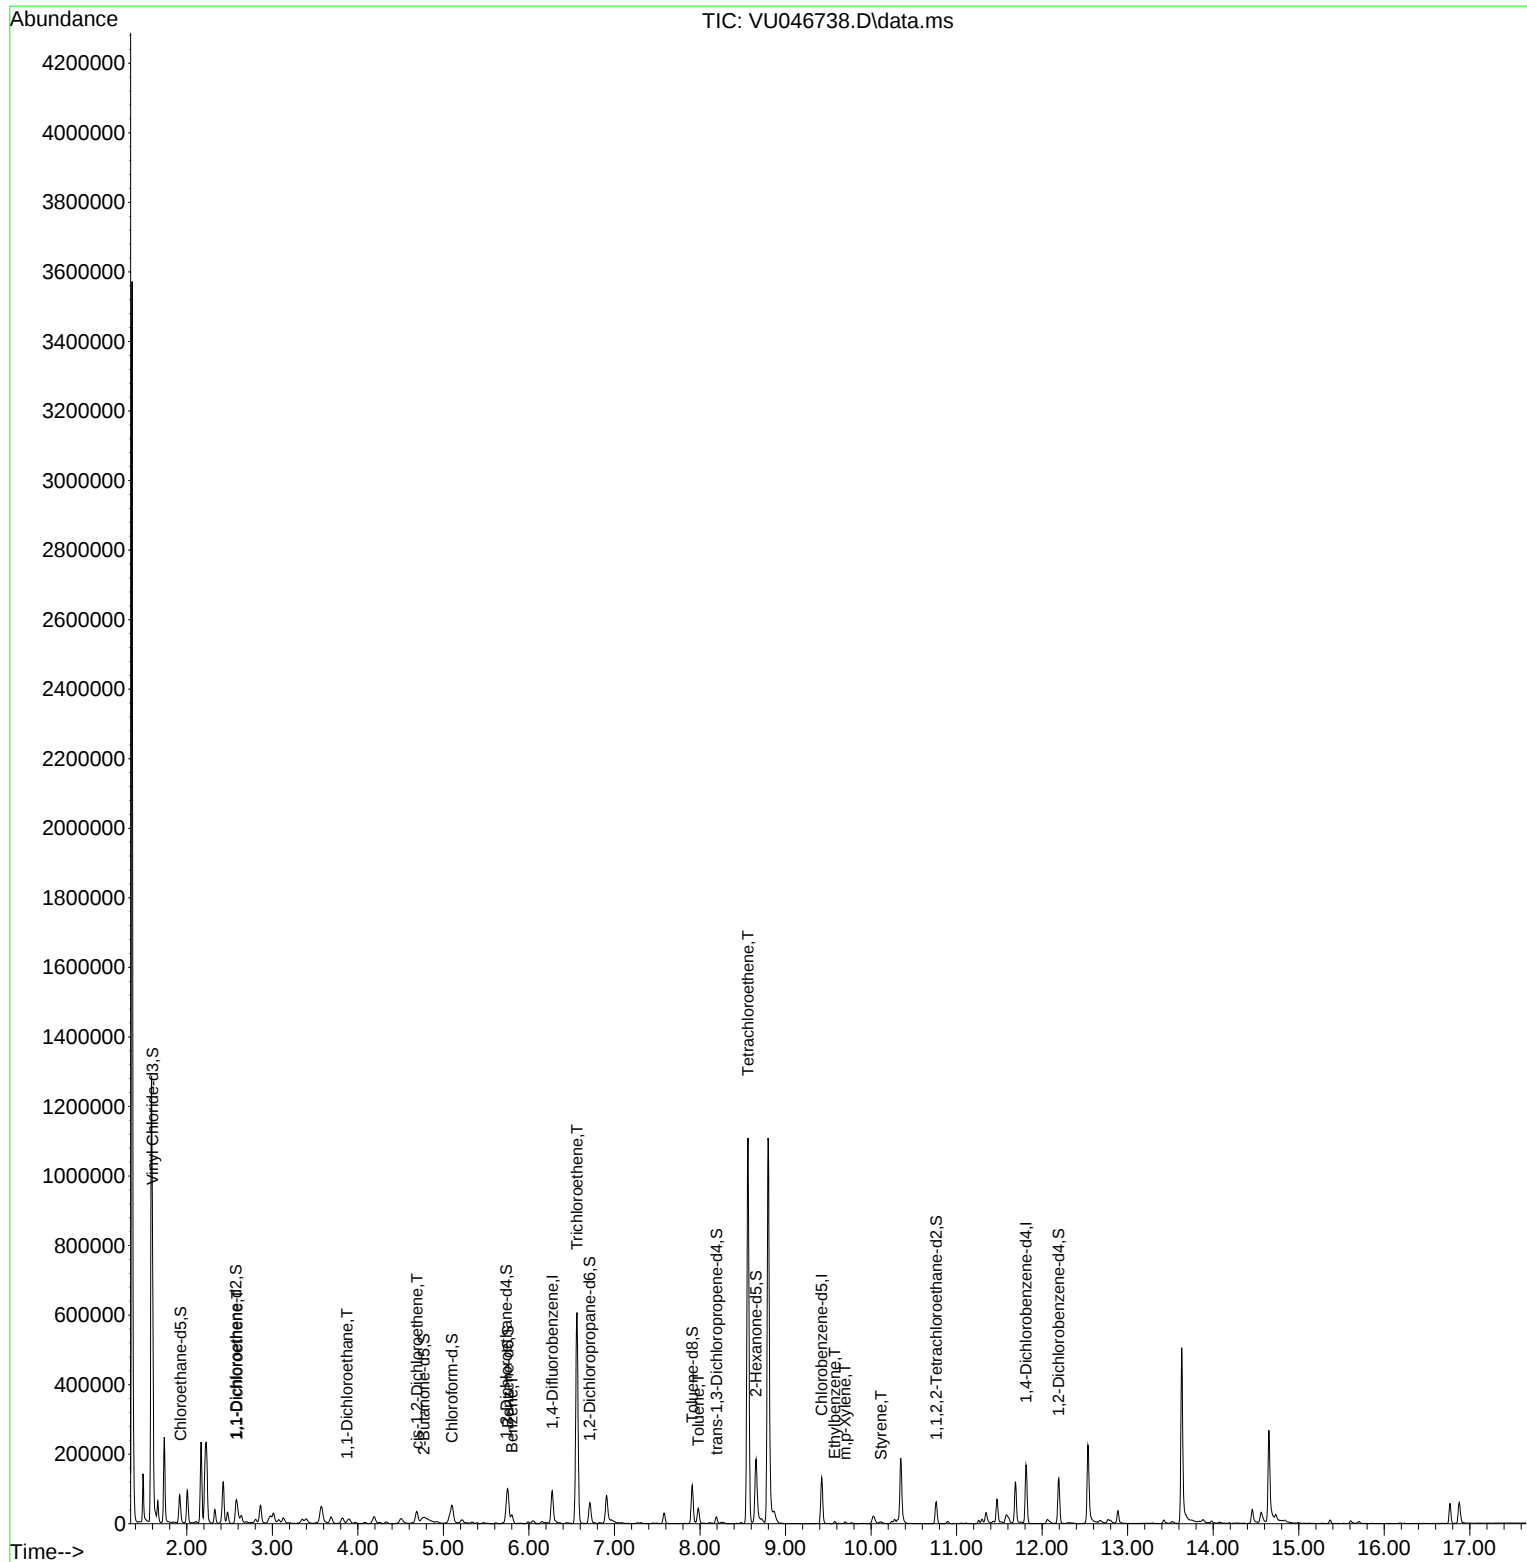




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011222\
Data File : VU046738.D
Acq On : 12 Jan 2022 13:28
Operator : SY/MD
Sample : N1101-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXW4

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/13/2022
Supervised By :Mahesh Dadoda 01/13/2022

Quant Time: Jan 12 13:44:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jan 10 00:25:50 2022
Response via : Initial Calibration

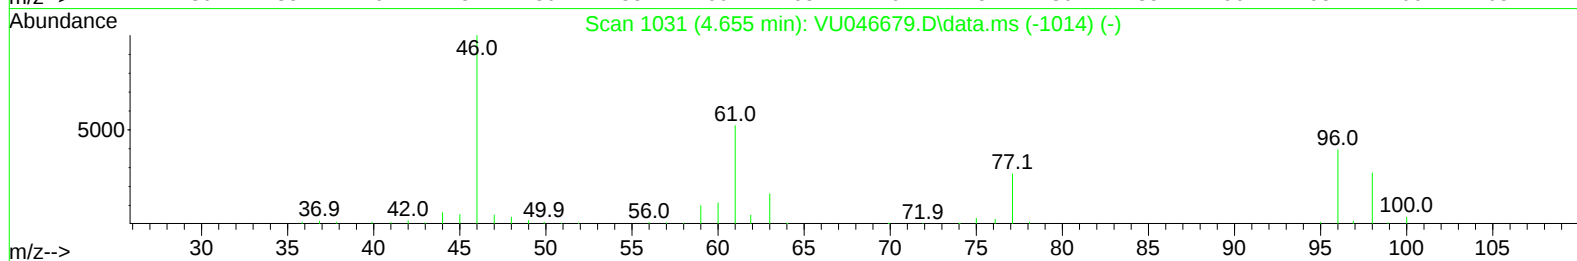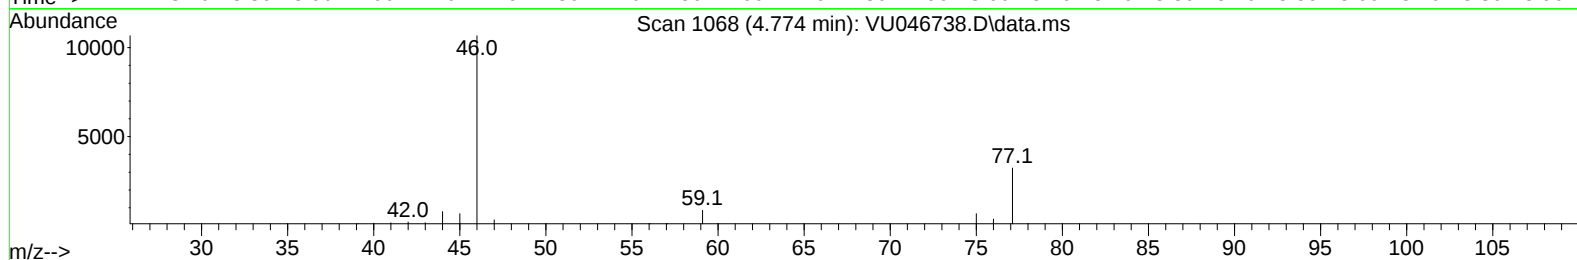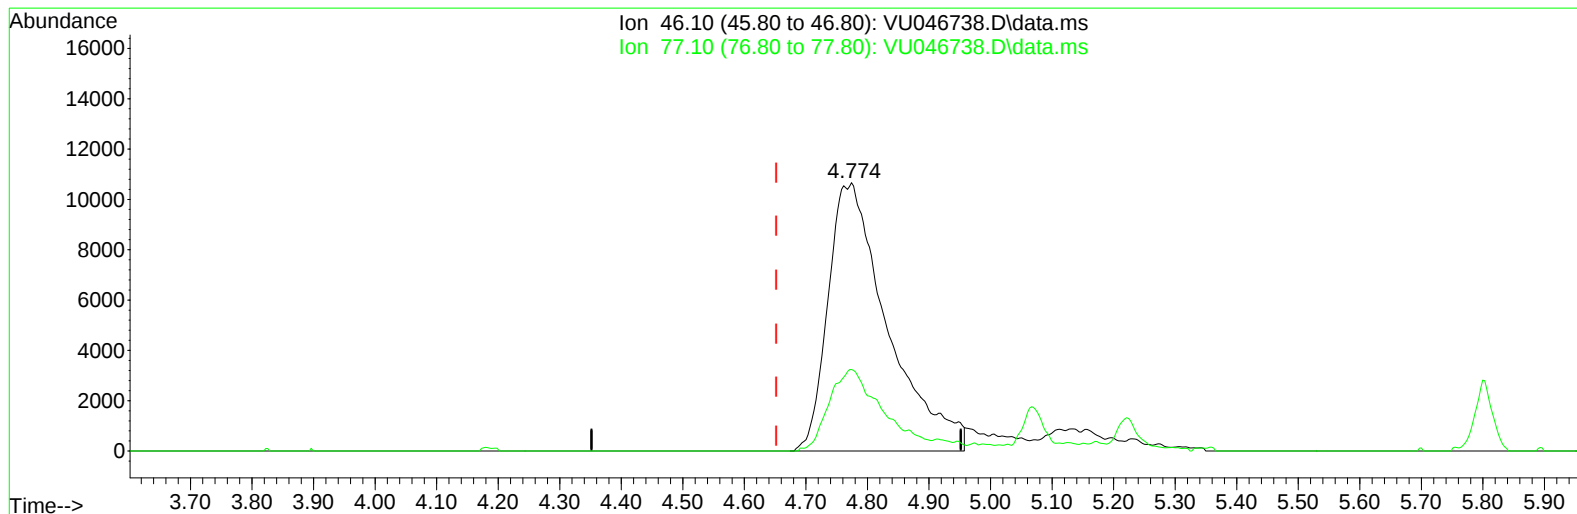

TIC: VU046738.D\data.ms

(20) 2-Butanone-d5 (S)

4.774min (+ 0.122) 40.47 ug/L m

response 71512

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	25.10	25.16
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011222\
Data File : VU046738.D
Acq On : 12 Jan 2022 13:28
Operator : SY/MD
Sample : N1101-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXW4

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/13/2022
Supervised By :Mahesh Dadoda 01/13/2022

Quant Time: Jan 12 13:44:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jan 10 00:25:50 2022
Response via : Initial Calibration

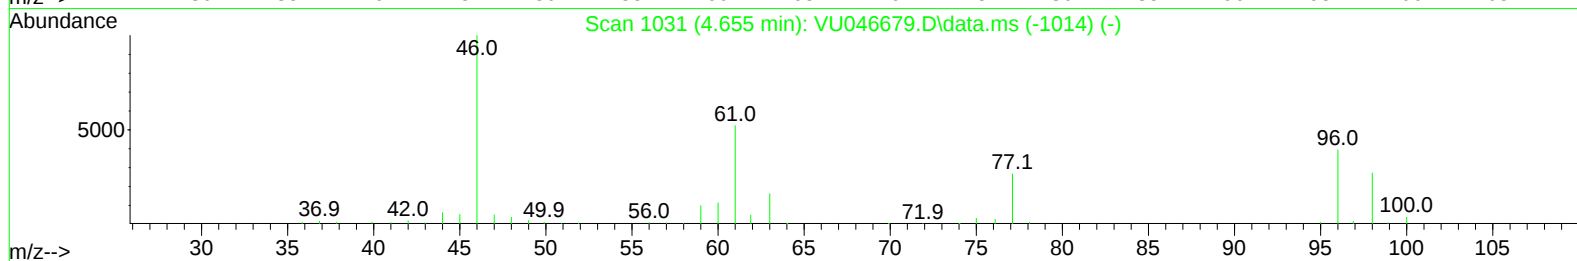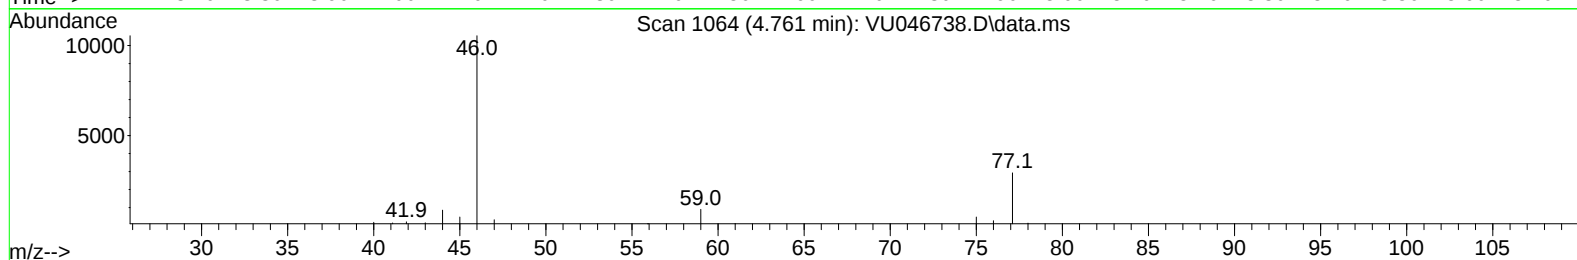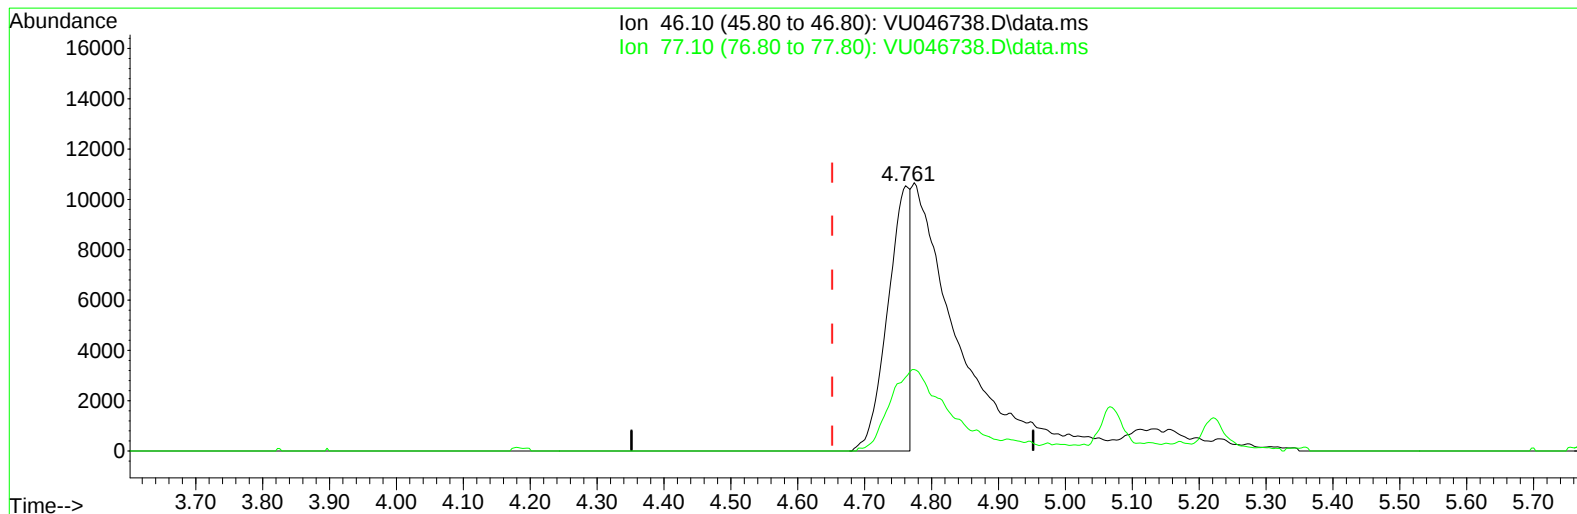

TIC: VU046738.D\data.ms

(20) 2-Butanone-d5 (S)

4.761min (+ 0.109) 13.75 ug/L

response 24300

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	25.10	74.05#
0.00	0.00	0.00
0.00	0.00	0.00