

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011222\
 Data File : VU046743.D
 Acq On : 12 Jan 2022 15:31
 Operator : SY/MD
 Sample : N1101-03DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXW6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU046743.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.363	3	7	18	rVB4	4587	5602	1.36%	0.189%
2	1.475	34	42	52	rBV	254066	247475	60.19%	8.330%
3	1.604	74	82	103	rVB	24227	34174	8.31%	1.150%
4	1.919	172	180	197	rBV	18682	30237	7.35%	1.018%
5	2.565	369	381	396	rVB2	50387	86912	21.14%	2.925%
6	3.047	522	531	543	rBV3	2631	5038	1.23%	0.170%
7	3.186	558	574	591	rBV2	7660	18646	4.53%	0.628%
8	3.369	619	631	645	rVB4	2504	5613	1.37%	0.189%
9	4.655	1011	1031	1075	rBV	39032	173166	42.12%	5.829%
10	5.067	1143	1159	1180	rVB	51360	114024	27.73%	3.838%
11	5.314	1224	1236	1249	rVB3	5725	12499	3.04%	0.421%
12	5.726	1344	1364	1388	rBV2	96003	252751	61.47%	8.507%
13	6.250	1513	1527	1546	rBV2	86257	162014	39.40%	5.453%
14	6.542	1610	1618	1627	rVB2	4946	8272	2.01%	0.278%
15	6.690	1652	1664	1679	rBV	62417	118539	28.83%	3.990%
16	7.568	1925	1937	1951	rBV	31482	55258	13.44%	1.860%
17	7.899	2026	2040	2055	rBV	112086	194878	47.40%	6.559%
18	8.182	2117	2128	2141	rBV	19535	34422	8.37%	1.159%
19	8.555	2232	2244	2259	rVB	89503	149830	36.44%	5.043%
20	8.655	2259	2275	2304	rBV	181128	411159	100.00%	13.839%
21	8.800	2309	2320	2338	rVB3	13260	28701	6.98%	0.966%
22	9.420	2501	2513	2533	rBV	128308	221712	53.92%	7.463%
23	10.764	2918	2931	2943	rBV2	70145	113111	27.51%	3.807%
24	10.893	2963	2971	2981	rBV	5252	8469	2.06%	0.285%
25	11.693	3211	3220	3229	rVB3	5884	8104	1.97%	0.273%
26	11.815	3246	3258	3276	rBV	152767	238166	57.93%	8.017%
27	12.195	3365	3376	3391	rVB	136098	213549	51.94%	7.188%
28	12.889	3583	3592	3605	rBV2	13220	18615	4.53%	0.627%




Sum of corrected areas: 2970936

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011222\
Data File : VU046743.D
Acq On : 12 Jan 2022 15:31
Operator : SY/MD
Sample : N1101-03DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXW6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

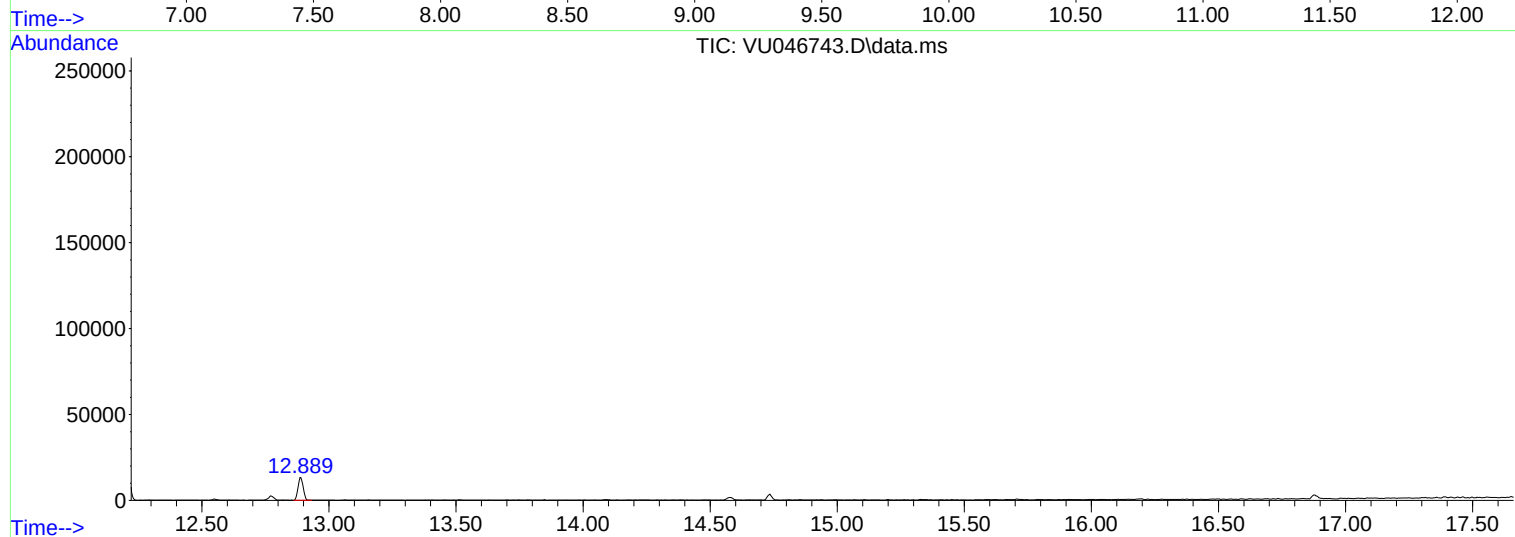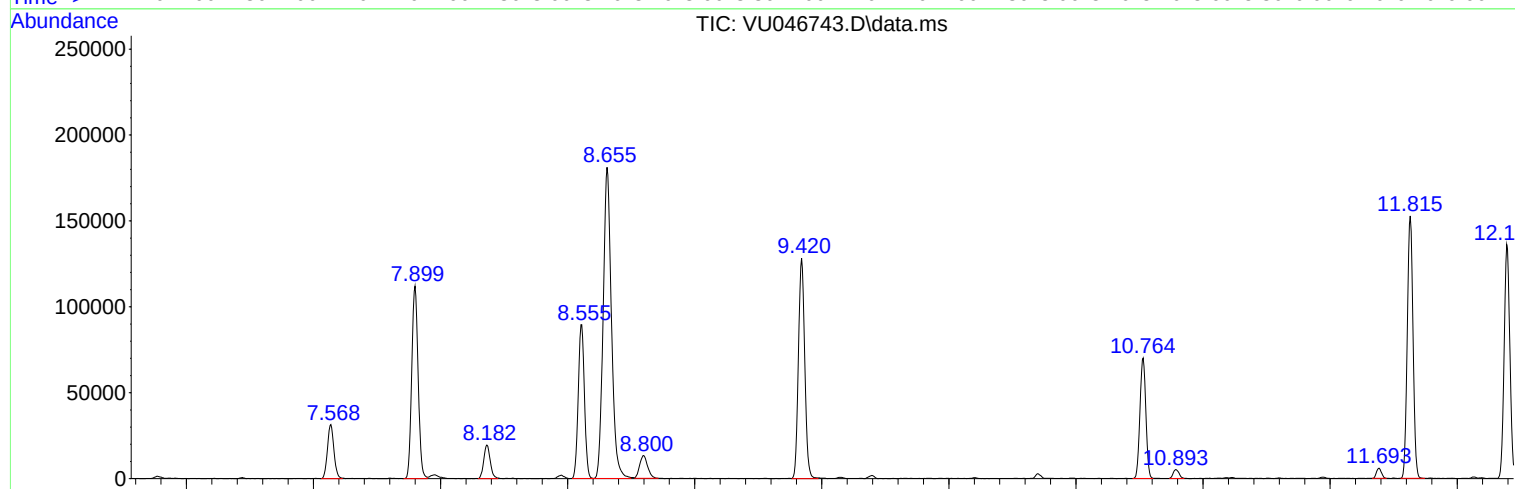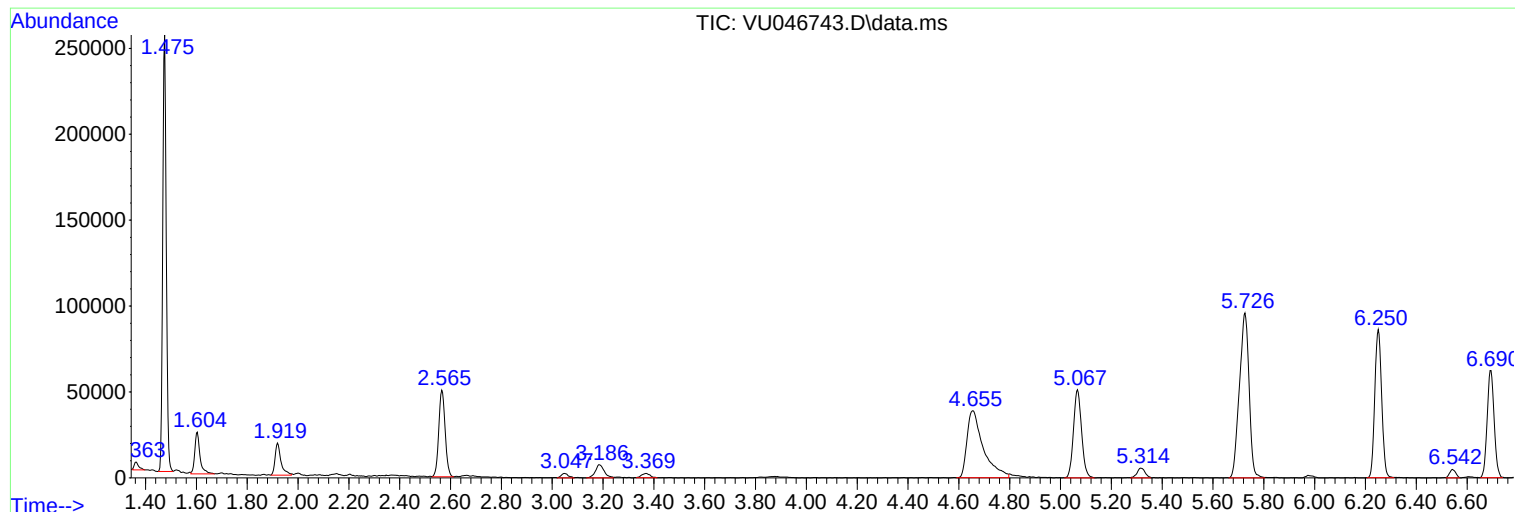

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011222\
Data File : VU046743.D
Acq On : 12 Jan 2022 15:31
Operator : SY/MD
Sample : N1101-03DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXW6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011222\
Data File : VU046743.D
Acq On : 12 Jan 2022 15:31
Operator : SY/MD
Sample : N1101-03DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXW6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc