


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011222\
 Data File : VU046733.D
 Acq On : 12 Jan 2022 09:18
 Operator : SY/MD
 Sample : BFB041
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB041

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Jan 10 00:25:50 2022

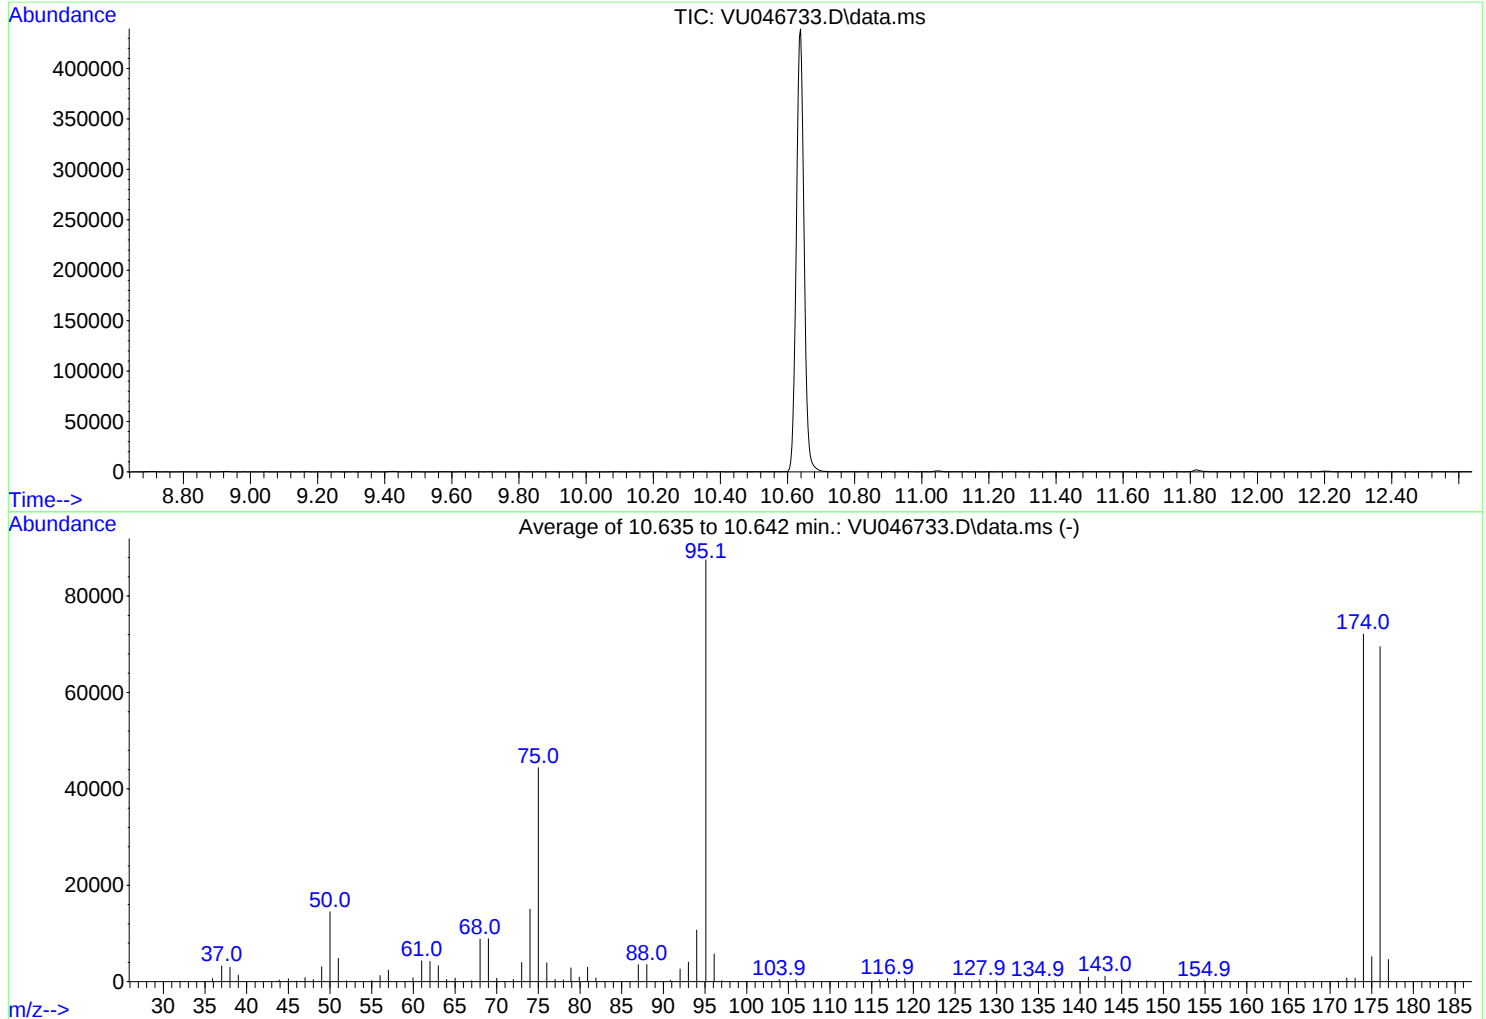

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	14511	PASS
75	95	30	80	50.7	44384	PASS
95	95	100	100	100.0	87509	PASS
96	95	5	9	6.6	5750	PASS
173	174	0.00	2	1.0	730	PASS
174	95	50	120	82.4	72107	PASS
175	174	5	9	7.2	5185	PASS
176	174	95	101	96.4	69499	PASS
177	176	5	9	6.6	4599	PASS

m/z	Abundance
36.00	109.0
43.90	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB041

m/z	Abundance
35.90	749.0
37.00	3467.0
38.00	3043.0
39.00	1366.0
44.00	506.0
45.00	675.0
45.90	139.0
47.00	893.0
48.00	430.0
49.00	3098.0
50.00	14872.0
51.00	5014.0
52.00	209.0
55.00	208.0
56.00	1223.0
57.00	2413.0
59.90	783.0
61.00	4696.0
62.00	4276.0
63.00	3369.0
64.00	479.0
65.00	788.0
67.00	227.0
68.00	9105.0
69.00	8924.0
70.00	727.0
72.00	490.0
73.00	4039.0
74.00	15336.0
75.00	45528.0
76.00	3939.0
77.00	505.0
78.00	353.0
78.90	2963.0
79.90	1003.0
80.90	3155.0
81.90	769.0
87.00	3467.0
88.00	3617.0
90.90	343.0
92.00	2637.0
93.00	4114.0
94.00	10938.0
95.10	88800.0
96.10	5962.0
97.00	215.0
103.90	444.0
104.90	106.0
105.90	437.0
106.90	111.0
115.90	443.0
116.90	642.0
118.00	410.0
118.90	654.0
127.90	364.0
128.90	144.0
129.90	299.0
130.90	122.0
135.00	160.0
136.90	190.0
141.00	900.0
141.90	137.0
143.00	1237.0
145.00	385.0
145.90	162.0
148.00	195.0
154.90	203.0
156.90	133.0
159.00	113.0
170.90	146.0
172.00	799.0
173.00	734.0
174.00	72304.0
175.00	5364.0
176.00	69608.0
177.00	4613.0

Instrument :
MSVOA_U
ClientSampleId :
BFB041

m/z	Abundance
35.00	766.0
37.00	3387.0
38.00	3088.0
39.00	1392.0
43.00	478.0
45.00	643.0
46.00	153.0
47.00	859.0
48.00	445.0
49.00	3219.0
50.00	14931.0
51.00	4966.0
52.00	197.0
55.00	235.0
56.00	1296.0
57.00	2448.0
60.00	841.0
61.00	4465.0
62.00	4381.0
63.00	3365.0
64.00	480.0
65.00	732.0
67.00	209.0
68.00	9170.0
69.00	9216.0
70.00	727.0
72.00	508.0
73.00	4132.0
74.00	15533.0
75.00	45832.0
76.00	4086.0
77.00	465.0
78.00	374.0
78.00	2933.0
79.00	980.0
80.00	3059.0
81.00	773.0
82.00	101.0
87.00	3637.0
88.00	3700.0
90.00	300.0
92.00	2724.0
93.00	4136.0
94.00	11051.0
95.00	90360.0
96.00	5928.0
97.00	211.0
103.00	447.0
104.00	113.0
105.00	426.0
106.00	100.0
111.00	109.0
114.00	106.0
115.00	410.0
116.00	684.0
118.00	417.0
118.00	610.0
127.00	375.0
128.00	161.0
129.00	320.0
130.00	111.0
135.00	133.0
136.00	214.0
141.00	953.0
142.00	135.0
143.00	1141.0
145.00	407.0
145.00	161.0
148.00	220.0
154.00	238.0
157.00	140.0
159.00	115.0
170.00	147.0
172.00	803.0
173.00	771.0
174.00	74448.0
175.00	5363.0
176.00	71664.0
177.00	4796.0

Instrument :
MSVOA_U
ClientSampleId :
BFB041

m/z	Abundance
35.90	715.0
37.00	2938.0
38.00	2788.0
39.00	1277.0
43.90	445.0
45.00	514.0
45.90	118.0
47.00	709.0
48.00	401.0
49.00	2916.0
50.00	13730.0
51.00	4420.0
52.00	186.0
55.00	217.0
56.00	1272.0
57.00	2179.0
60.00	781.0
61.00	3814.0
62.00	3884.0
63.00	3097.0
64.00	429.0
65.00	645.0
66.90	206.0
68.00	8183.0
69.00	8576.0
70.00	656.0
72.00	513.0
73.00	3786.0
74.00	14139.0
75.00	41792.0
76.00	3751.0
77.00	404.0
78.00	349.0
78.90	2709.0
79.90	832.0
80.90	2751.0
81.90	749.0
87.00	3469.0
88.00	3337.0
90.80	269.0
92.00	2553.0
93.00	3870.0
94.00	10123.0
95.10	83368.0
96.10	5361.0
97.00	180.0
103.90	371.0
105.00	116.0
105.90	387.0
111.00	110.0
114.90	110.0
115.90	365.0
116.90	662.0
117.90	374.0
119.00	521.0
127.90	336.0
128.90	146.0
129.90	309.0
131.00	115.0
134.90	118.0
136.90	189.0
141.00	933.0
142.00	127.0
143.00	969.0
145.00	338.0
146.00	135.0
148.00	236.0
149.90	109.0
154.90	248.0
157.00	172.0
170.90	133.0
172.00	742.0
173.00	686.0
174.00	69568.0
175.00	4827.0
176.00	67224.0
177.00	4389.0

Instrument :
MSVOA_U
ClientSampleId :
BFB041