


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011322\
Data File : VU046750.D
Acq On : 13 Jan 2022 09:46
Operator : SY/MD
Sample : BFB042
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB042

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Jan 10 00:25:50 2022

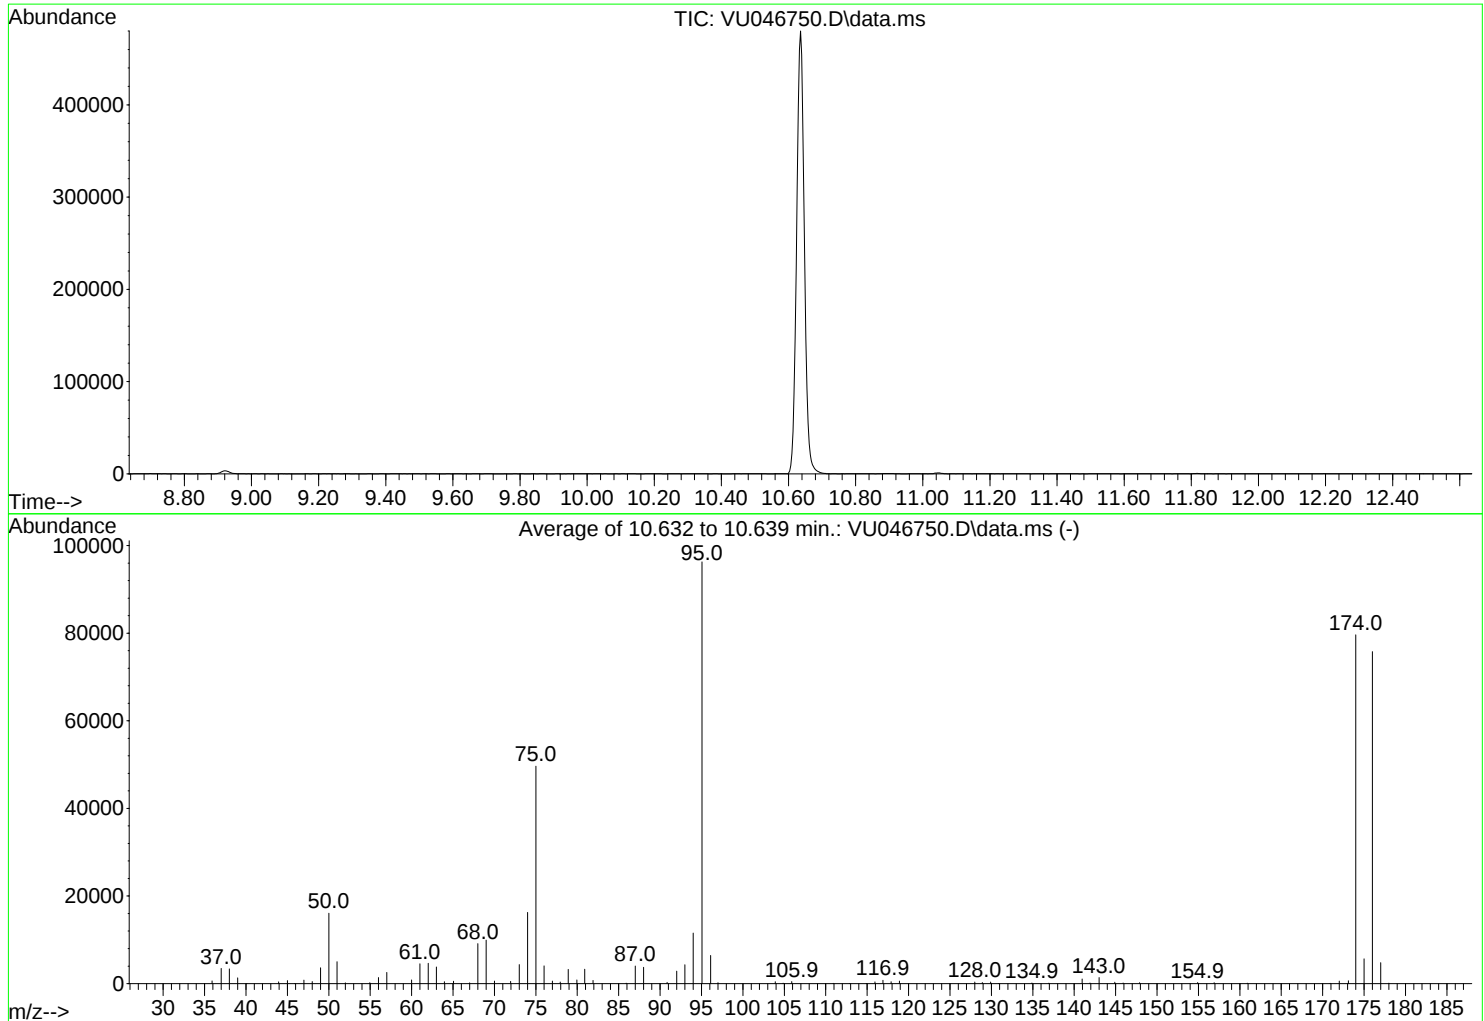

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.7	16060	PASS
75	95	30	80	51.6	49643	PASS
95	95	100	100	100.0	96288	PASS
96	95	5	9	6.7	6418	PASS
173	174	0.00	2	0.8	644	PASS
174	95	50	120	82.7	79608	PASS
175	174	5	9	7.1	5662	PASS
176	174	95	101	95.2	75784	PASS
177	176	5	9	6.3	4806	PASS

m/z	Abundance
43.90	120.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042

m/z	Abundance
35.90	646.0
37.00	3472.0
38.00	3410.0
39.00	1402.0
40.10	100.0
44.00	472.0
45.00	710.0
45.90	100.0
47.00	835.0
48.00	480.0
49.00	3636.0
50.00	16248.0
51.00	5225.0
52.00	175.0
55.00	228.0
56.00	1357.0
57.00	2617.0
60.00	835.0
61.00	4656.0
62.00	4647.0
63.00	3851.0
64.00	476.0
65.10	579.0
67.00	192.0
68.00	9431.0
69.00	9957.0
70.00	578.0
72.00	492.0
73.00	4249.0
74.00	16093.0
75.00	49432.0
76.00	4112.0
77.00	571.0
78.00	399.0
78.90	3382.0
79.90	814.0
80.90	3273.0
81.90	749.0
85.90	104.0
87.00	3861.0
88.00	3741.0
90.90	340.0
92.00	2791.0
93.00	4257.0
94.00	11357.0
95.00	95584.0
96.10	6365.0
97.00	235.0
103.90	486.0
104.90	152.0
105.90	446.0
110.90	122.0
114.90	102.0
115.90	357.0
116.90	773.0
117.90	468.0
118.90	553.0
128.00	342.0
128.90	259.0
129.90	358.0
135.00	154.0
137.00	135.0
141.00	1075.0
141.90	124.0
143.00	1388.0
144.90	330.0
145.90	167.0
147.90	243.0
154.90	250.0
156.90	208.0
160.90	108.0
170.90	126.0
172.00	546.0
173.10	618.0
174.00	76656.0
175.00	5554.0
176.00	73944.0
177.00	4778.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042

m/z	Abundance
35.90	628.0
37.00	3578.0
38.00	3471.0
39.00	1342.0
44.00	555.0
45.00	712.0
47.00	826.0
48.00	504.0
49.00	3762.0
50.00	16624.0
51.00	5142.0
52.00	169.0
55.00	226.0
56.00	1434.0
57.00	2647.0
60.00	865.0
61.00	4697.0
62.00	4833.0
63.00	3943.0
63.90	449.0
65.00	547.0
67.00	204.0
68.00	9397.0
69.00	10258.0
70.00	573.0
72.00	537.0
73.00	4553.0
74.00	16760.0
75.00	51280.0
76.00	4218.0
77.00	598.0
77.90	389.0
78.90	3345.0
80.00	860.0
80.90	3387.0
81.90	744.0
85.90	138.0
87.00	4229.0
88.00	3862.0
90.80	292.0
92.00	2933.0
93.00	4454.0
94.00	11930.0
95.00	99400.0
96.10	6706.0
97.00	229.0
103.90	457.0
104.80	129.0
105.90	514.0
110.90	110.0
115.90	418.0
116.90	788.0
117.90	472.0
118.90	596.0
128.00	378.0
128.90	260.0
129.90	370.0
134.90	153.0
137.00	120.0
141.00	1079.0
141.90	149.0
143.00	1447.0
144.90	321.0
145.90	151.0
147.90	236.0
154.90	258.0
156.90	251.0
160.90	107.0
170.90	106.0
172.00	618.0
173.10	662.0
174.00	82384.0
175.00	5869.0
176.00	78304.0
177.00	4944.0
178.00	137.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042

m/z	Abundance
35.90	602.0
37.00	3339.0
38.00	3179.0
39.00	1213.0
44.00	573.0
45.00	631.0
47.00	781.0
48.00	474.0
49.00	3436.0
50.00	15309.0
51.00	4620.0
52.00	174.0
54.90	215.0
56.00	1344.0
57.00	2400.0
60.00	810.0
61.00	4238.0
62.00	4489.0
63.00	3648.0
63.90	418.0
65.00	507.0
67.00	192.0
68.00	8581.0
69.00	9621.0
70.00	562.0
71.90	491.0
73.00	4251.0
74.00	15910.0
75.00	48216.0
76.00	3815.0
77.00	574.0
77.90	359.0
78.90	2990.0
80.00	841.0
80.90	3201.0
81.90	677.0
85.90	151.0
87.00	3987.0
88.00	3624.0
90.90	288.0
92.00	2796.0
93.00	4210.0
94.00	11367.0
95.10	93880.0
96.10	6183.0
97.00	177.0
103.90	376.0
104.80	103.0
105.90	484.0
112.90	103.0
116.00	425.0
116.90	717.0
117.90	435.0
118.90	602.0
128.00	379.0
128.90	214.0
129.90	334.0
130.90	109.0
134.80	140.0
136.90	123.0
140.90	1005.0
141.90	134.0
143.00	1369.0
144.90	285.0
145.90	137.0
147.90	200.0
154.90	245.0
156.90	246.0
160.90	100.0
172.00	644.0
173.10	653.0
174.00	79784.0
175.00	5562.0
176.00	75104.0
177.00	4697.0
178.00	167.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042