


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU011420\
 Data File : VU036447.D
 Acq On : 14 Jan 2020 13:21
 Operator : JC/MD
 Sample : BFB39
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB39

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM011420WMA.M
 Title : VOC Analysis
 Last Update : Wed Jan 15 00:18:03 2020

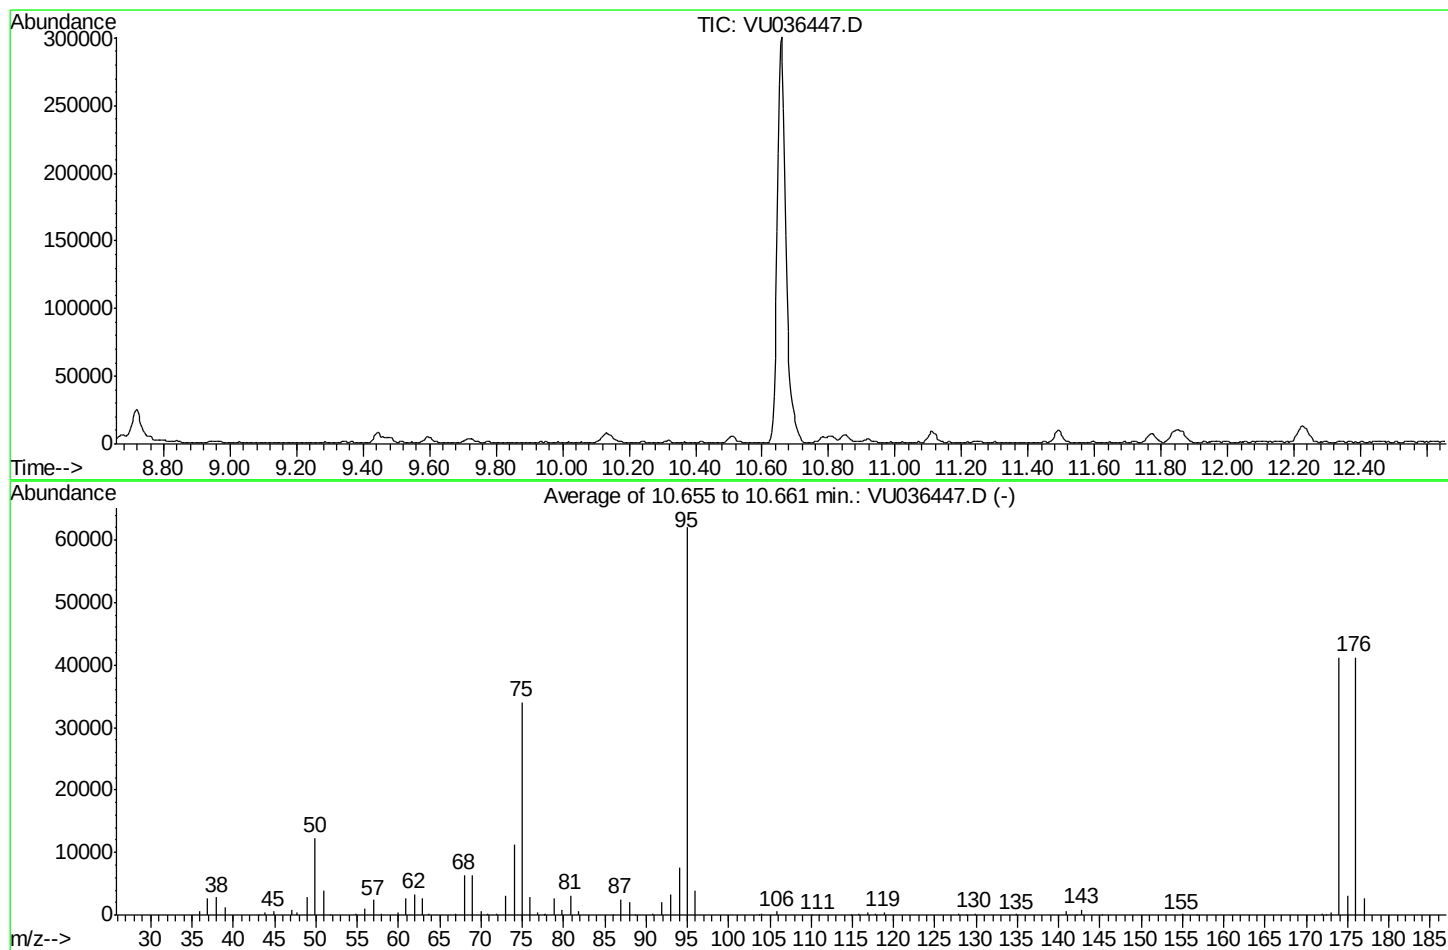

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2885

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	12390	PASS
75	95	30	80	54.9	34069	PASS
95	95	100	100	100.0	62037	PASS
96	95	5	9	6.4	3950	PASS
173	174	0.00	2	1.0	408	PASS
174	95	50	120	66.4	41213	PASS
175	174	5	9	7.3	3002	PASS
176	174	95	101	100.1	41240	PASS
177	176	5	9	6.3	2583	PASS

m/z	Abundance
35.80	543.0
36.90	3063.0
38.00	2847.0
38.90	1477.0
43.90	1063.0
44.90	511.0
47.00	630.0
47.70	487.0
48.90	3040.0
49.90	12615.0
51.00	3553.0
51.80	113.0
54.80	275.0
55.90	1221.0
57.00	2322.0
57.90	144.0
60.00	359.0
60.90	2717.0
61.90	3254.0
62.90	2505.0
63.70	219.0
66.90	220.0
68.00	6428.0
68.90	6784.0
70.00	670.0
70.80	205.0
72.00	364.0
73.00	3040.0
74.00	11906.0
75.00	34728.0
76.00	2836.0
76.80	471.0
77.90	366.0
78.80	2865.0
79.80	733.0
80.90	3143.0
81.80	636.0
86.90	2601.0
87.90	2226.0
90.90	366.0
91.90	2133.0
93.00	2949.0
94.00	7914.0
95.00	62896.0
95.90	3921.0
104.00	267.0
105.90	434.0
110.00	130.0
114.80	125.0
115.80	211.0
116.80	431.0
117.80	215.0
118.80	474.0
127.90	185.0
129.90	283.0
134.90	123.0
140.90	717.0
142.80	788.0
155.00	106.0
156.70	139.0
172.00	170.0
173.00	328.0
173.90	41216.0
174.90	2888.0
175.90	41176.0
176.90	2595.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

m/z	Abundance
35.80	608.0
36.90	2775.0
38.00	2949.0
38.90	1254.0
40.00	134.0
43.90	1035.0
44.90	548.0
47.10	883.0
47.80	424.0
48.90	2991.0
49.90	12586.0
51.00	3990.0
54.80	256.0
55.90	1090.0
57.00	2469.0
57.90	190.0
59.90	473.0
61.00	2687.0
61.90	3563.0
63.00	2759.0
67.00	151.0
68.00	6594.0
68.90	6546.0
70.00	572.0
70.80	147.0
71.90	277.0
73.00	3271.0
74.00	11581.0
75.00	34744.0
76.00	2949.0
76.80	442.0
77.80	200.0
78.80	2835.0
79.80	869.0
80.90	3250.0
81.80	727.0
86.90	2592.0
88.00	2022.0
88.70	138.0
90.90	242.0
91.90	2125.0
93.00	3351.0
94.00	7660.0
95.00	63584.0
95.90	4009.0
104.00	236.0
105.90	583.0
114.80	111.0
115.80	197.0
116.80	472.0
117.80	245.0
118.80	530.0
127.90	179.0
129.90	261.0
134.90	217.0
140.90	773.0
142.10	113.0
142.80	855.0
145.20	141.0
155.00	163.0
172.00	206.0
172.40	225.0
173.00	433.0
173.90	42136.0
175.00	3062.0
175.90	42424.0
177.00	2651.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

m/z	Abundance
35.90	584.0
36.90	2395.0
38.00	2612.0
39.00	960.0
39.90	227.0
43.00	125.0
43.90	905.0
44.90	596.0
47.10	758.0
47.80	420.0
48.90	2476.0
50.00	11970.0
50.90	3926.0
54.80	192.0
56.00	945.0
57.00	2317.0
58.00	187.0
59.80	626.0
61.00	2651.0
61.90	3253.0
63.00	2630.0
63.70	236.0
67.10	118.0
68.00	6334.0
69.00	5830.0
70.00	485.0
71.90	278.0
73.00	2993.0
74.00	10543.0
75.00	32736.0
76.00	2867.0
76.80	289.0
77.60	145.0
78.80	2612.0
79.80	893.0
80.80	3134.0
81.80	684.0
86.00	207.0
86.90	2236.0
88.00	1665.0
88.70	191.0
90.70	259.0
91.80	1770.0
93.00	3264.0
94.00	7060.0
95.00	59632.0
95.90	3920.0
103.70	256.0
105.90	589.0
110.90	115.0
115.90	205.0
116.80	490.0
117.90	248.0
118.80	487.0
127.90	164.0
128.80	157.0
129.80	228.0
134.90	267.0
140.90	666.0
142.80	847.0
145.20	110.0
155.00	147.0
171.90	237.0
173.00	465.0
174.00	40288.0
175.00	3058.0
175.90	40120.0
177.00	2505.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39

Scan 2885 (10.616 min): VU036447.D
BFB39

m/z	Abundance
39.80	131.0
43.90	585.0
54.80	118.0
72.90	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB39