

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011722\
 Data File : VU046763.D
 Acq On : 17 Jan 2022 13:36
 Operator : SY/MD
 Sample : VU0117WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK063

Quant Time: Jan 18 02:16:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 18 02:15:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	200759	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	195421	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	93693	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	72023	41.112	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.220%
7) Chloroethane-d5	1.916	69	55729	42.821	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.640%
11) 1,1-Dichloroethene-d2	2.572	63	91989	30.873	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	61.740%
21) 2-Butanone-d5	4.636	46	110563	86.230	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	86.230%
24) Chloroform-d	5.067	84	127242	41.201	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.400%
26) 1,2-Dichloroethane-d4	5.703	65	85410	43.607	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.220%
32) Benzene-d6	5.729	84	268235	43.983	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.960%
36) 1,2-Dichloropropane-d6	6.690	67	82366	44.264	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	88.520%
41) Toluene-d8	7.899	98	248185	45.522	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.040%
43) trans-1,3-Dichloroprop...	8.182	79	42479	47.384	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.760%
47) 2-Hexanone-d5	8.636	63	93121	94.199	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	94.200%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	127000	44.068	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.140%
66) 1,2-Dichlorobenzene-d4	12.195	152	97452	50.266	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.540%
Target Compounds						
13) Acetone	2.655	43	2591	2.123	ug/L	50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011722\
Data File : VU046763.D
Acq On : 17 Jan 2022 13:36
Operator : SY/MD
Sample : VU0117WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK063

Quant Time: Jan 18 02:16:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 18 02:15:56 2022
Response via : Initial Calibration

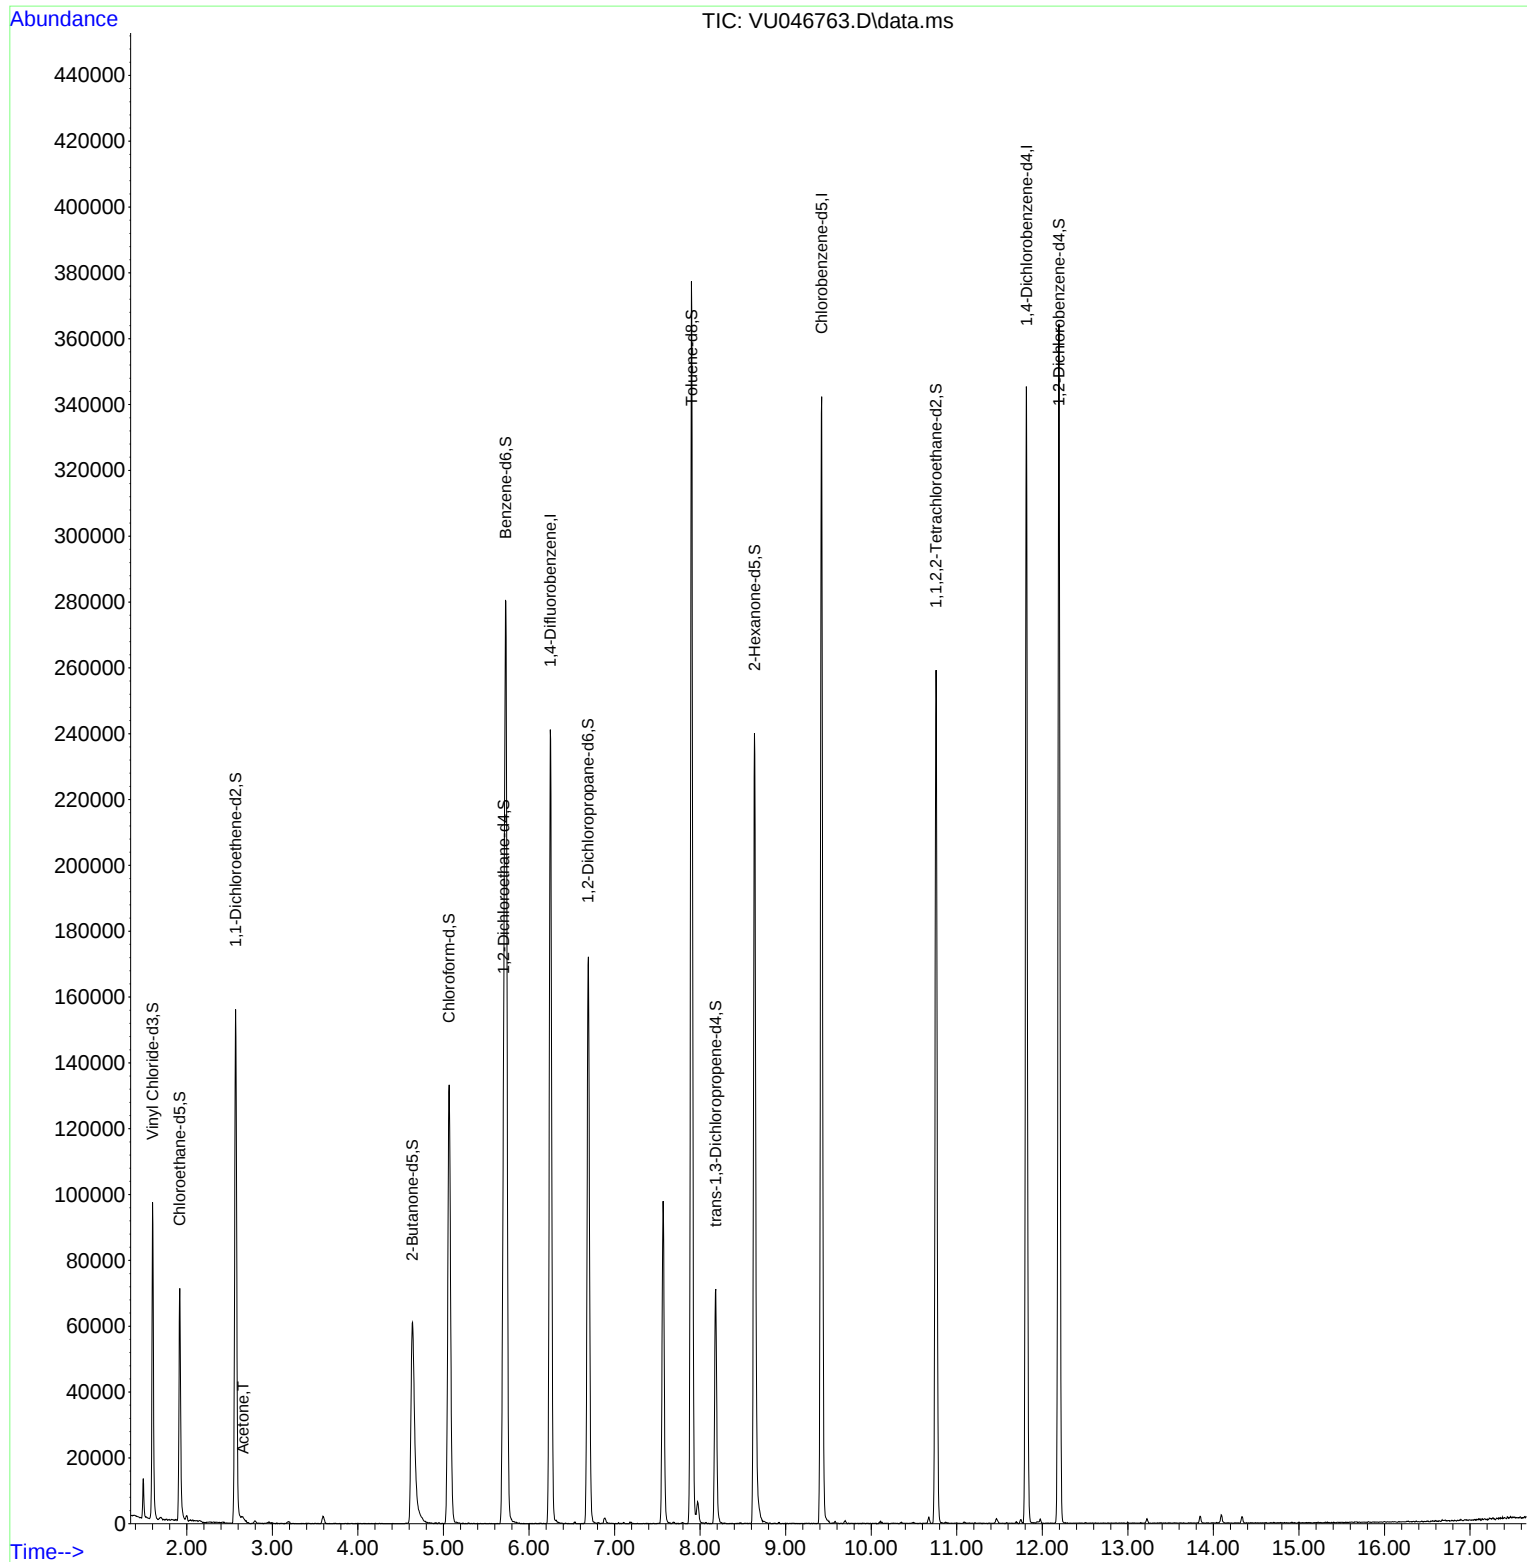

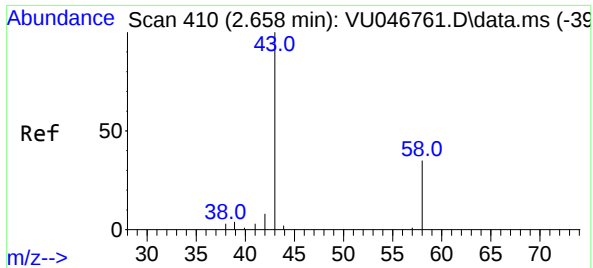

#13
 Acetone
 Concen: 2.123 ug/L
 RT: 2.655 min Scan# 409
 Delta R.T. -0.003 min
 Lab File: VU046763.D
 Acq: 17 Jan 2022 13:36

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK063

Tgt Ion: 43 Resp: 2591
 Ion Ratio Lower Upper
 43 100
 58 6.0 0.0 71.0

