

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011722\
 Data File : VU046762.D
 Acq On : 17 Jan 2022 13:01
 Operator : SY/MD
 Sample : VU0117MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK062

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Title : VOC Analysis

Signal : TIC: VU046762.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.472	35	41	51	rVB	33329	34104	4.63%	0.572%
2	1.601	73	81	101	rVB	92709	107621	14.61%	1.805%
3	1.919	170	180	204	rVB	67246	93238	12.65%	1.563%
4	2.572	370	383	400	rBV	149502	247461	33.58%	4.149%
5	2.797	444	453	463	rVB2	1527	2772	0.38%	0.046%
6	2.864	463	474	477	rBV2	366	751	0.10%	0.013%
7	2.925	491	493	495	rBV	242	163	0.02%	0.003%
8	3.080	539	541	547	rVB2	224	226	0.03%	0.004%
9	3.109	548	550	556	rVB2	212	164	0.02%	0.003%
10	3.179	567	572	573	rBV	585	479	0.07%	0.008%
11	3.353	622	626	630	rBV2	460	525	0.07%	0.009%
12	3.559	686	690	693	rBB	139	142	0.02%	0.002%
13	4.183	881	884	888	rBB	118	127	0.02%	0.002%
14	4.639	1011	1026	1069	rBV	58280	189835	25.76%	3.183%
15	4.912	1109	1111	1114	rVV2	253	167	0.02%	0.003%
16	4.929	1114	1116	1119	rVB2	285	180	0.02%	0.003%
17	5.067	1143	1159	1176	rBV	132261	292630	39.71%	4.907%
18	5.501	1289	1294	1297	rBB	131	157	0.02%	0.003%
19	5.726	1343	1364	1392	rBV2	272775	736830	100.00%	12.355%
20	5.912	1419	1422	1425	rBV	147	131	0.02%	0.002%
21	5.932	1425	1428	1431	rVB2	265	217	0.03%	0.004%
22	6.250	1512	1527	1546	rVV	241002	447903	60.79%	7.510%
23	6.539	1609	1617	1623	rBB4	816	1102	0.15%	0.018%
24	6.691	1651	1664	1680	rBV	168160	322387	43.75%	5.406%
25	6.781	1691	1692	1696	rVB	358	149	0.02%	0.002%
26	6.813	1699	1702	1708	rBV2	292	391	0.05%	0.007%
27	6.925	1734	1737	1741	rBB	164	158	0.02%	0.003%
28	7.041	1770	1773	1777	rBB	239	164	0.02%	0.003%
29	7.105	1791	1793	1795	rVB	229	130	0.02%	0.002%
30	7.189	1814	1819	1824	rVB2	446	505	0.07%	0.008%
31	7.350	1863	1869	1872	rBB	129	183	0.02%	0.003%
32	7.372	1873	1876	1880	rBV	151	167	0.02%	0.003%
33	7.411	1885	1888	1891	rBB	147	131	0.02%	0.002%
34	7.565	1924	1936	1956	rBV	95185	170147	23.09%	2.853%
35	7.655	1962	1964	1969	rVB2	255	234	0.03%	0.004%
36	7.691	1969	1975	1979	rBV2	345	487	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011722\
 Data File : VU046762.D
 Acq On : 17 Jan 2022 13:01
 Operator : SY/MD
 Sample : VU0117MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK062

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Title : VOC Analysis

37	7.800	2002	2009	2016	rVB2	529	761	0.10%	0.013%
38	7.900	2026	2040	2055	rBV	358890	611558	83.00%	10.254%
39	7.973	2057	2063	2075	rVB2	5401	8553	1.16%	0.143%
40	8.179	2116	2127	2146	rVV	69706	116184	15.77%	1.948%
41	8.269	2152	2155	2158	rVB3	320	209	0.03%	0.004%
42	8.404	2193	2197	2199	rBV2	217	167	0.02%	0.003%
43	8.472	2207	2218	2227	rBB2	1275	2353	0.32%	0.039%
44	8.549	2239	2242	2247	rBV2	623	555	0.08%	0.009%
45	8.636	2256	2269	2297	rBV	244010	431175	58.52%	7.230%
46	8.957	2364	2369	2372	rBV	173	214	0.03%	0.004%
47	9.035	2390	2393	2396	rBV	158	133	0.02%	0.002%
48	9.227	2450	2453	2458	rBB	151	173	0.02%	0.003%
49	9.263	2461	2464	2467	rBB	165	130	0.02%	0.002%
50	9.346	2487	2490	2493	rBV	136	141	0.02%	0.002%
51	9.417	2498	2512	2534	rBV	337601	557412	75.65%	9.346%
52	9.571	2553	2560	2569	rVB2	1057	1817	0.25%	0.030%
53	9.697	2591	2599	2606	rBV2	1333	1983	0.27%	0.033%
54	9.764	2615	2620	2624	rBV	145	220	0.03%	0.004%
55	9.899	2659	2662	2665	rBV	156	157	0.02%	0.003%
56	10.025	2698	2701	2703	rBV	172	147	0.02%	0.002%
57	10.108	2718	2727	2736	rVB6	1857	2790	0.38%	0.047%
58	10.292	2781	2784	2789	rBV	171	190	0.03%	0.003%
59	10.353	2800	2803	2807	rBB	190	183	0.02%	0.003%
60	10.395	2812	2816	2822	rBV	160	264	0.04%	0.004%
61	10.485	2838	2844	2852	rBB3	1058	1498	0.20%	0.025%
62	10.536	2858	2860	2864	rBV	133	145	0.02%	0.002%
63	10.584	2871	2875	2877	rBV	135	134	0.02%	0.002%
64	10.620	2882	2886	2893	rBB	156	250	0.03%	0.004%
65	10.671	2894	2902	2910	rBV2	1751	2379	0.32%	0.040%
66	10.758	2915	2929	2945	rBV	254797	404030	54.83%	6.775%
67	10.819	2945	2948	2953	rBV3	724	601	0.08%	0.010%
68	10.880	2959	2967	2968	rBV	507	543	0.07%	0.009%
69	10.896	2968	2972	2978	rVB3	1189	1359	0.18%	0.023%
70	10.986	2993	3000	3002	rBV	169	240	0.03%	0.004%
71	11.044	3013	3018	3022	rBB	183	218	0.03%	0.004%
72	11.083	3023	3030	3031	rBV	1066	864	0.12%	0.014%
73	11.472	3139	3151	3160	rVB4	2226	3649	0.50%	0.061%
74	11.578	3180	3184	3189	rBV2	335	401	0.05%	0.007%
75	11.697	3215	3221	3226	rVV2	690	777	0.11%	0.013%
76	11.745	3229	3236	3245	rVV5	2700	4081	0.55%	0.068%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011722\
 Data File : VU046762.D
 Acq On : 17 Jan 2022 13:01
 Operator : SY/MD
 Sample : VU0117MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK062

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
 Title : VOC Analysis

77	11.813	3245	3257	3279	rVV	338735	537397	72.93%	9.011%
78	11.915	3285	3289	3290	rVV	189	136	0.02%	0.002%
79	11.944	3291	3298	3301	rVV2	493	618	0.08%	0.010%
80	11.970	3301	3306	3314	rVB2	1163	1571	0.21%	0.026%
81	12.067	3332	3336	3338	rBV2	244	235	0.03%	0.004%
82	12.195	3359	3376	3398	rBV	347099	566453	76.88%	9.498%
83	12.501	3465	3471	3476	rBV	126	162	0.02%	0.003%
84	12.639	3511	3514	3520	rVB	321	235	0.03%	0.004%
85	12.774	3552	3556	3559	rVB2	216	185	0.03%	0.003%
86	12.999	3620	3626	3632	rVB3	858	1230	0.17%	0.021%
87	13.221	3687	3695	3705	rVB2	3849	5881	0.80%	0.099%
88	13.845	3880	3889	3897	rVB3	6470	9348	1.27%	0.157%
89	14.089	3955	3965	3980	rBV2	10146	16441	2.23%	0.276%
90	14.144	3980	3982	3986	rVV2	215	175	0.02%	0.003%
91	14.333	4031	4041	4050	rBV	7510	10777	1.46%	0.181%
92	14.472	4079	4084	4087	rBV	173	172	0.02%	0.003%
93	15.275	4331	4334	4338	rBV	174	134	0.02%	0.002%
94	15.430	4379	4382	4385	rBV2	201	187	0.03%	0.003%
95	15.681	4455	4460	4464	rBV2	249	329	0.04%	0.006%
96	16.262	4639	4641	4645	rBV2	239	157	0.02%	0.003%
97	16.340	4662	4665	4667	rBV	249	153	0.02%	0.003%
98	16.523	4719	4722	4727	rBV2	273	176	0.02%	0.003%
99	16.555	4727	4732	4735	rBV3	301	334	0.05%	0.006%
100	17.041	4878	4883	4886	rBV3	539	614	0.08%	0.010%




Sum of corrected areas: 5963896

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011722\
Data File : VU046762.D
Acq On : 17 Jan 2022 13:01
Operator : SY/MD
Sample : VU0117MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK062

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

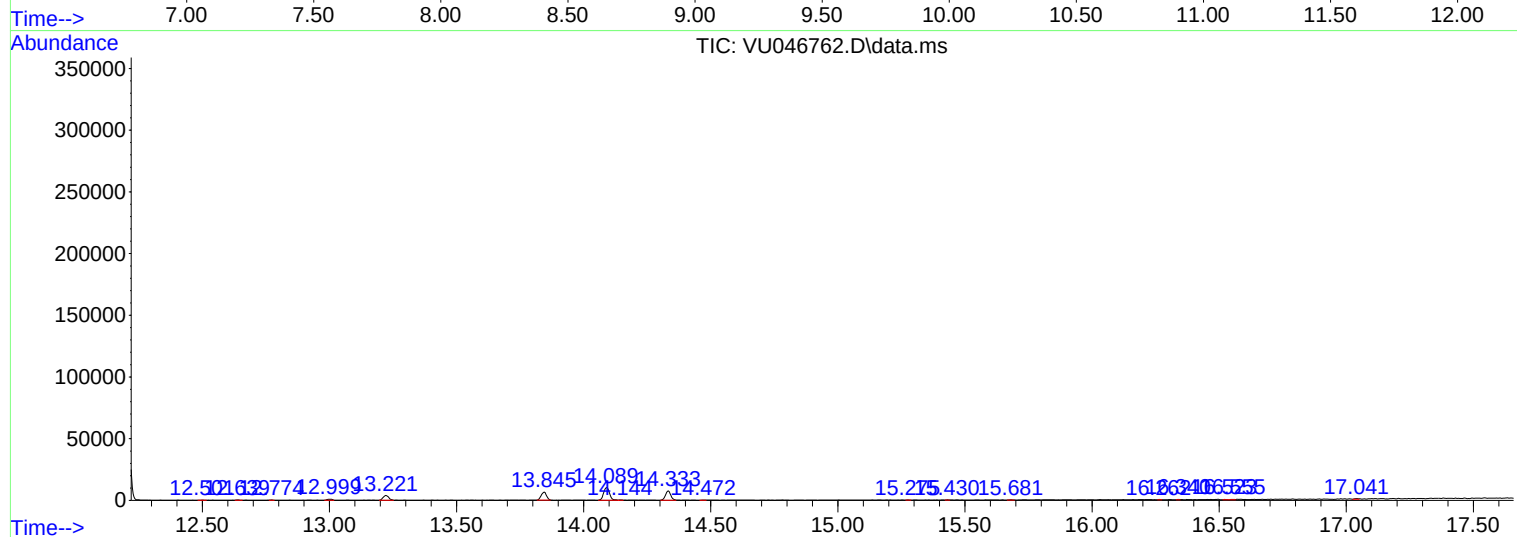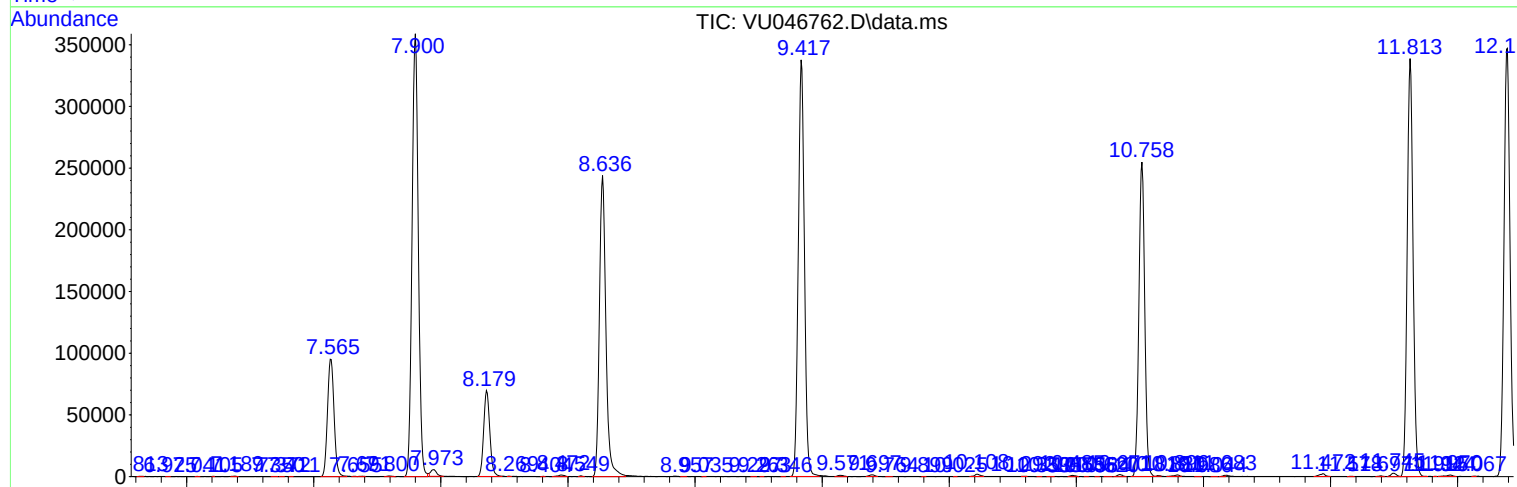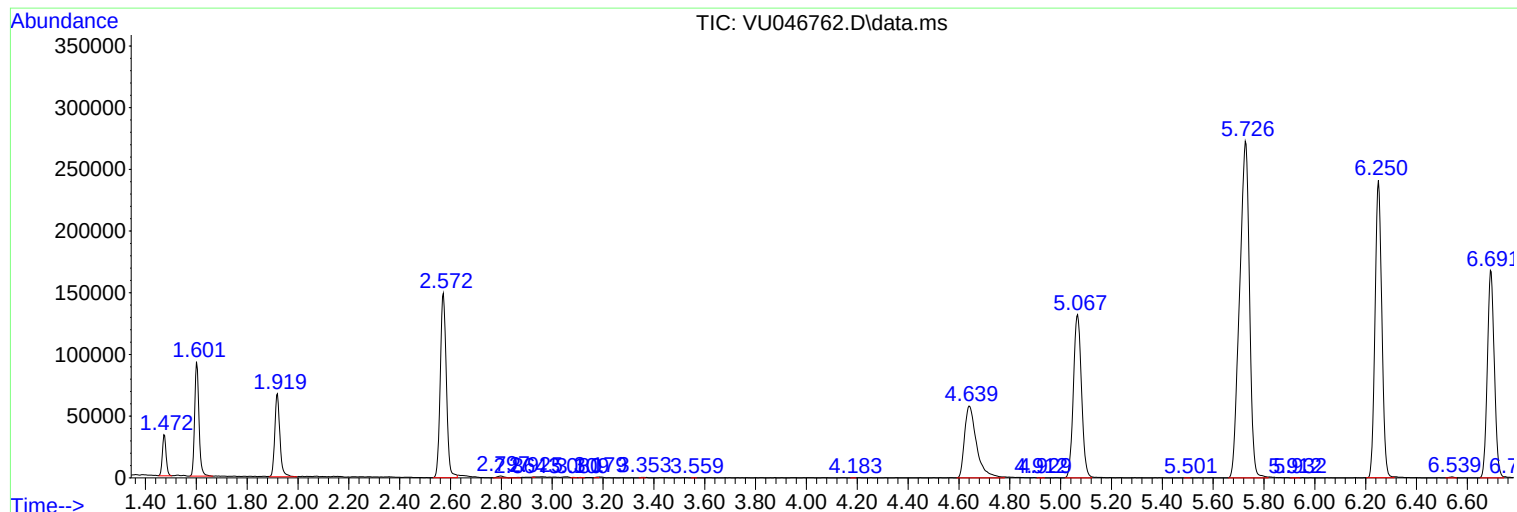

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011722\
Data File : VU046762.D
Acq On : 17 Jan 2022 13:01
Operator : SY/MD
Sample : VU0117MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK062

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011722\
Data File : VU046762.D
Acq On : 17 Jan 2022 13:01
Operator : SY/MD
Sample : VU0117MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK062

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
