


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011722\
Data File : VU046760.D
Acq On : 17 Jan 2022 09:02
Operator : SY/MD
Sample : BFB042
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB042

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM010522WMA.M
Title : VOC Analysis
Last Update : Tue Jan 18 02:15:56 2022

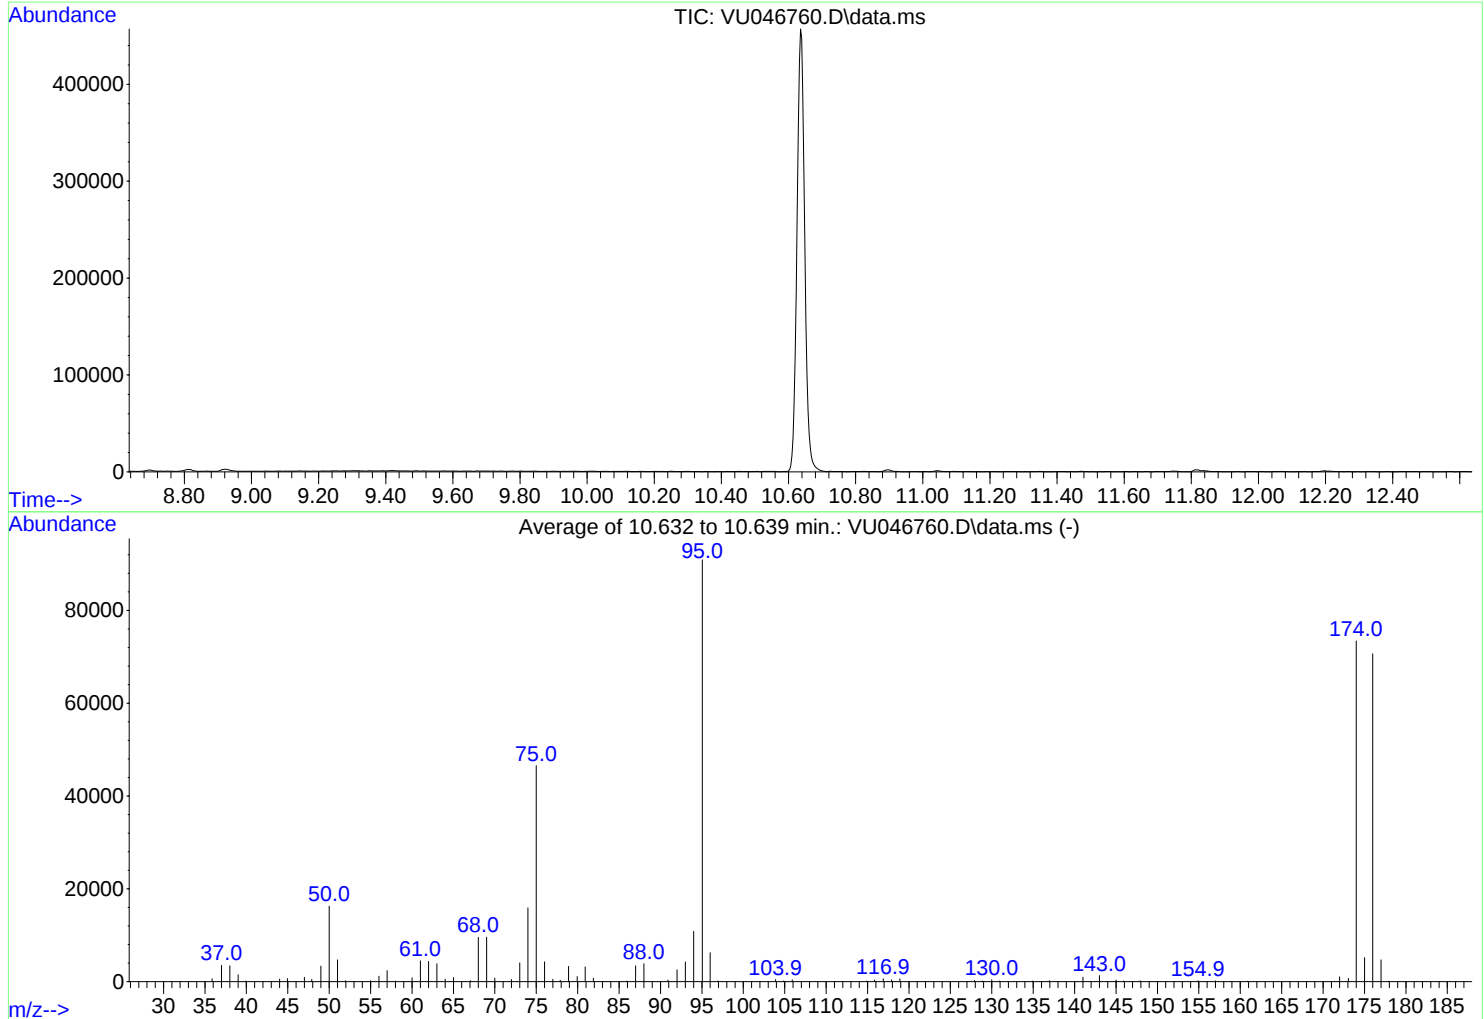

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	16277	PASS
75	95	30	80	51.2	46552	PASS
95	95	100	100	100.0	90891	PASS
96	95	5	9	6.9	6233	PASS
173	174	0.00	2	0.9	681	PASS
174	95	50	120	80.8	73397	PASS
175	174	5	9	7.0	5165	PASS
176	174	95	101	96.3	70659	PASS
177	176	5	9	6.6	4680	PASS

m/z	Abundance
35.90	763.0
37.00	3426.0
38.00	3359.0
39.00	1481.0
40.00	145.0
44.00	542.0
45.00	623.0
47.00	913.0
47.90	469.0
49.00	3233.0
50.00	15820.0
51.00	4547.0
51.90	204.0
53.00	102.0
55.00	220.0
56.00	1174.0
57.00	2256.0
58.00	149.0
60.00	798.0
61.00	4422.0
62.00	4313.0
63.00	3848.0
64.00	582.0
65.00	841.0
67.00	213.0
68.00	9390.0
69.00	9156.0
70.00	718.0
72.00	395.0
73.00	3908.0
74.00	15346.0
75.00	45128.0
76.00	4271.0
77.00	536.0
77.90	294.0
78.90	3165.0
80.00	1021.0
80.90	3183.0
81.90	697.0
86.00	164.0
87.00	3443.0
88.00	3812.0
90.90	327.0
92.00	2385.0
93.00	3948.0
94.00	10521.0
95.10	87160.0
96.00	6107.0
97.00	163.0
103.90	432.0
104.90	109.0
105.90	339.0
114.90	146.0
115.80	332.0
116.90	548.0
117.90	372.0
118.90	634.0
127.90	211.0
128.80	119.0
130.00	409.0
130.90	161.0
134.90	139.0
136.90	178.0
141.00	884.0
143.00	1308.0
145.00	332.0
145.80	127.0
147.90	147.0
154.90	176.0
157.00	160.0
160.90	102.0
171.00	126.0
172.00	991.0
173.10	745.0
174.00	68696.0
175.00	4987.0
176.00	65280.0
177.00	4606.0
178.00	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042

m/z	Abundance
35.90	221.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042

m/z	Abundance
35.90	896.0
37.00	3510.0
38.00	3364.0
39.00	1475.0
39.90	130.0
44.00	524.0
44.90	654.0
47.00	913.0
47.90	507.0
49.00	3334.0
50.00	16108.0
51.00	4718.0
52.00	192.0
55.00	202.0
56.00	1194.0
57.00	2423.0
58.00	134.0
60.00	873.0
61.00	4391.0
62.00	4210.0
63.00	3742.0
64.00	501.0
65.00	827.0
67.10	180.0
68.00	9418.0
69.00	9568.0
70.00	735.0
72.00	497.0
73.00	4115.0
74.00	15827.0
75.00	46432.0
76.00	4155.0
77.00	495.0
77.90	314.0
78.90	3275.0
79.90	1128.0
80.90	3082.0
81.90	716.0
85.80	122.0
87.00	3301.0
88.00	3789.0
90.90	349.0
92.00	2643.0
93.00	4407.0
94.00	10865.0
95.00	91512.0
96.00	6092.0
96.90	140.0
103.90	465.0
104.80	147.0
105.90	391.0
114.90	135.0
115.90	349.0
116.90	688.0
117.90	369.0
118.90	560.0
127.90	257.0
128.90	170.0
130.00	408.0
130.90	146.0
134.90	172.0
137.00	225.0
141.00	1047.0
141.90	124.0
143.00	1294.0
143.90	108.0
145.00	384.0
146.00	112.0
147.90	259.0
154.90	227.0
157.00	149.0
158.80	100.0
160.90	135.0
172.00	1052.0
173.00	622.0
174.00	75904.0
175.00	5173.0
176.00	73744.0
177.00	4587.0
177.90	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042

m/z	Abundance
35.90	865.0
37.00	3660.0
38.00	3522.0
39.00	1536.0
39.90	153.0
44.00	554.0
44.90	662.0
47.00	986.0
47.90	522.0
49.00	3452.0
50.00	16904.0
51.00	4847.0
52.00	204.0
55.00	244.0
56.00	1182.0
57.00	2421.0
58.00	158.0
60.00	861.0
61.00	4652.0
62.00	4513.0
63.00	4007.0
64.00	596.0
65.00	895.0
67.10	209.0
68.00	9884.0
69.00	9994.0
70.00	788.0
72.00	462.0
73.00	4136.0
74.00	16488.0
75.00	48096.0
76.00	4412.0
77.00	535.0
77.90	309.0
78.90	3385.0
79.90	1114.0
80.90	3252.0
81.90	736.0
86.00	151.0
87.00	3479.0
88.00	3992.0
90.90	349.0
92.00	2646.0
93.00	4397.0
94.00	11147.0
95.10	94000.0
96.00	6501.0
97.00	180.0
103.90	484.0
104.90	124.0
105.90	388.0
114.90	163.0
115.90	346.0
116.90	627.0
117.90	393.0
118.90	631.0
127.90	237.0
128.90	161.0
130.00	430.0
130.90	165.0
134.90	155.0
137.00	212.0
141.00	993.0
141.90	114.0
143.00	1343.0
143.90	109.0
145.00	371.0
145.90	133.0
147.90	217.0
154.90	189.0
157.00	172.0
160.90	127.0
171.00	116.0
172.00	1067.0
173.10	677.0
174.00	75592.0
175.00	5336.0
176.00	72952.0
177.00	4847.0
177.90	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042