


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012022\
Data File : VU046803.D
Acq On : 20 Jan 2022 11:40
Operator : SY/MD
Sample : VU0120WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK052

Manual IntegrationsAPPROVED

Quant Time: Jan 20 14:42:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 20 02:00:32 2022
Response via : Initial Calibration

Reviewed By :John Carlone 01/21/2022
Supervised By :Mahesh Dadoda 01/21/2022

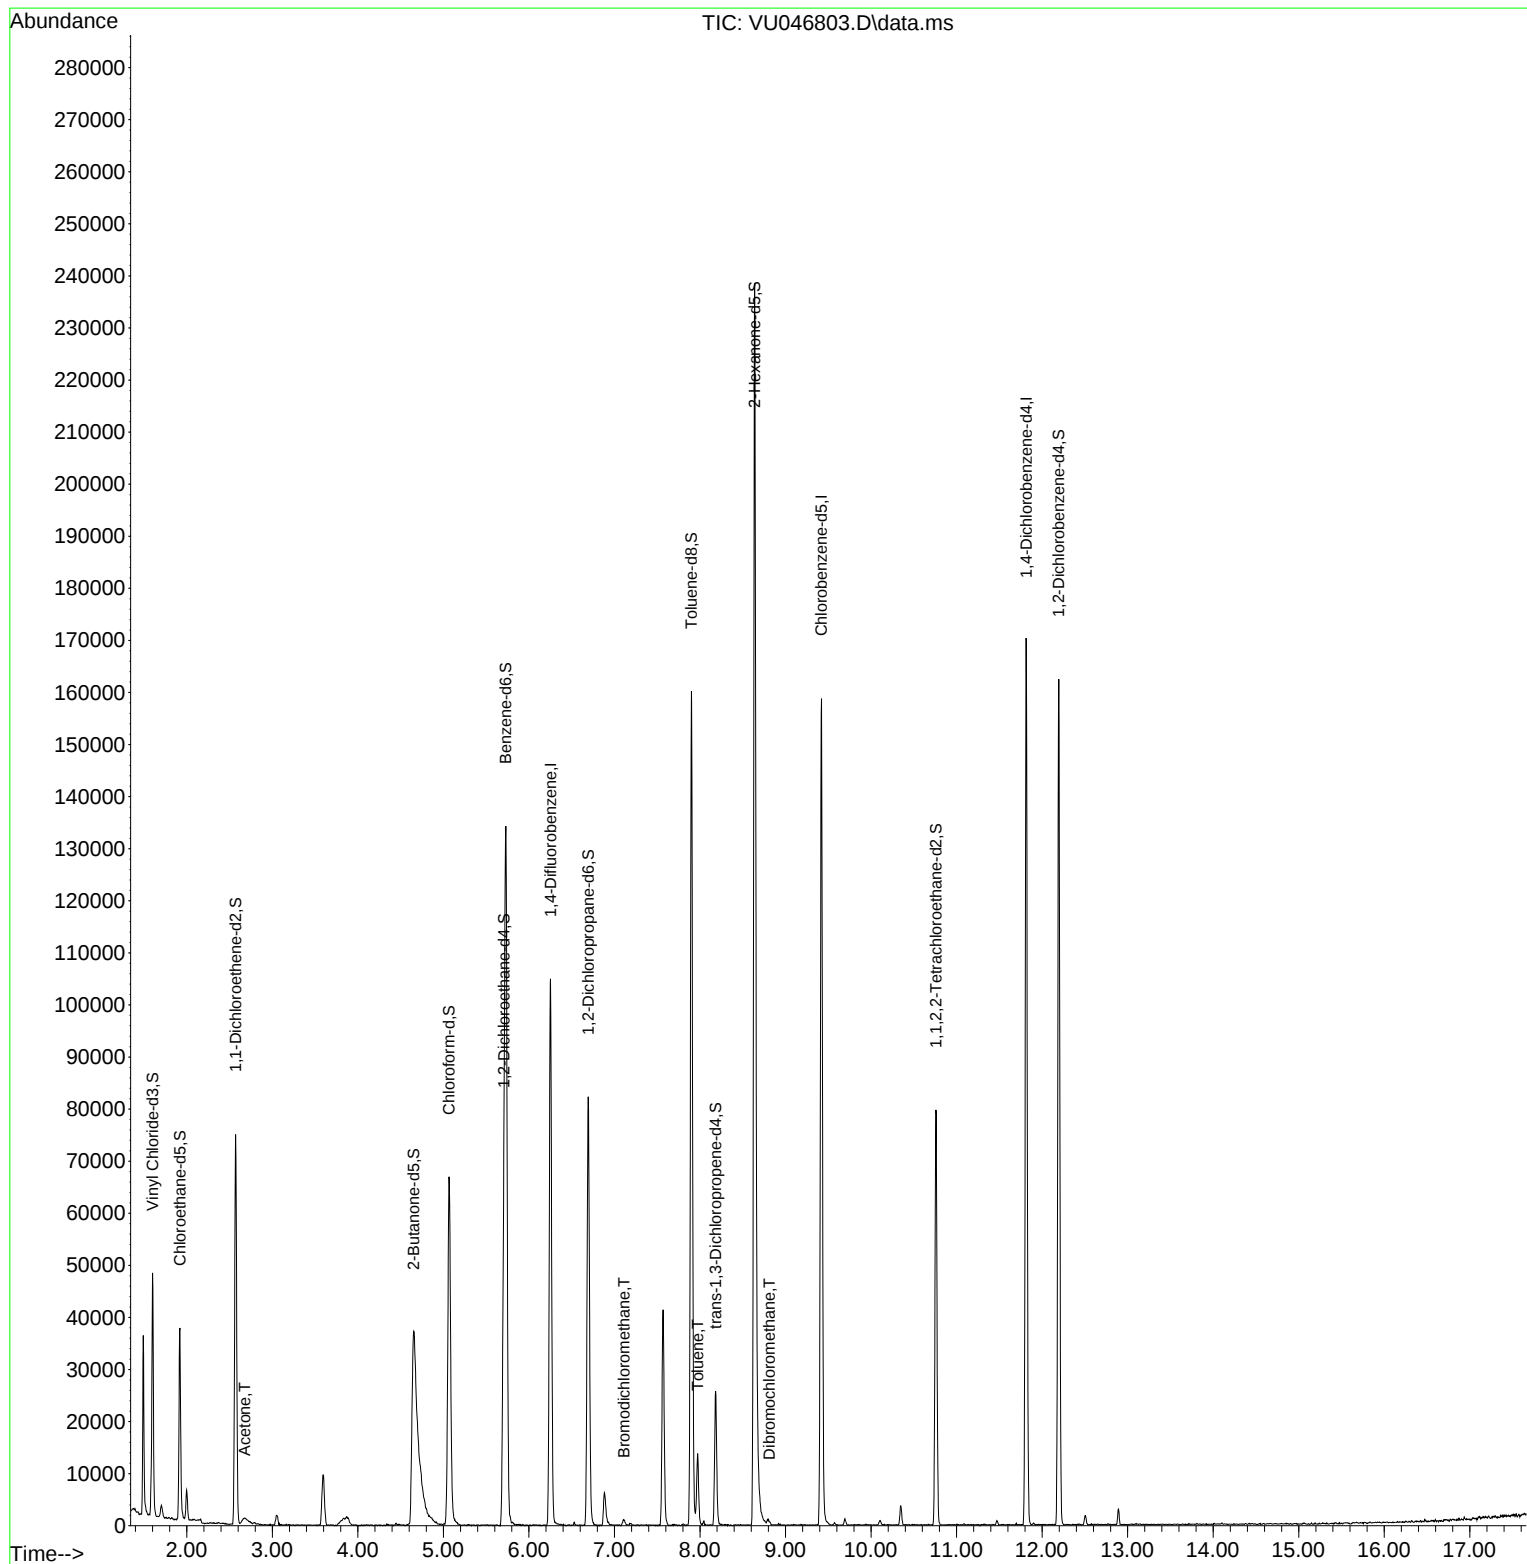




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012022\
Data File : VU046803.D
Acq On : 20 Jan 2022 11:40
Operator : SY/MD
Sample : VU0120WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK052

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/21/2022
Supervised By :Mahesh Dadoda 01/21/2022

Quant Time: Jan 20 14:42:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 20 02:00:32 2022
Response via : Initial Calibration

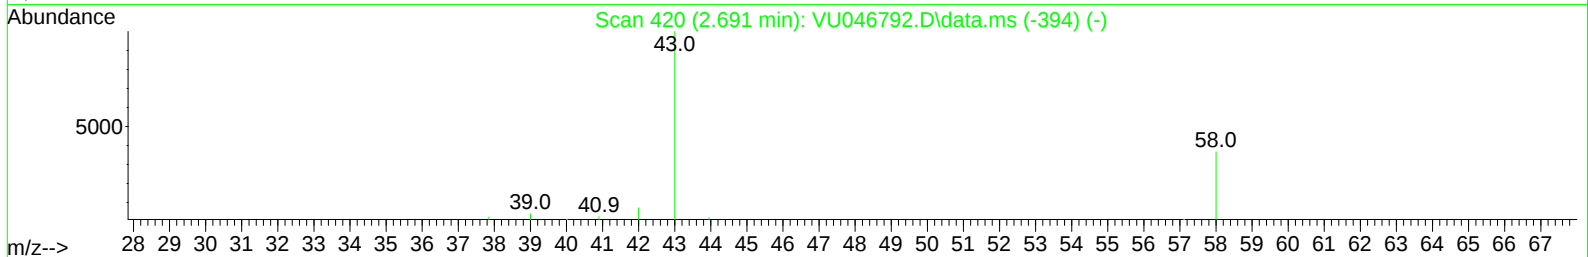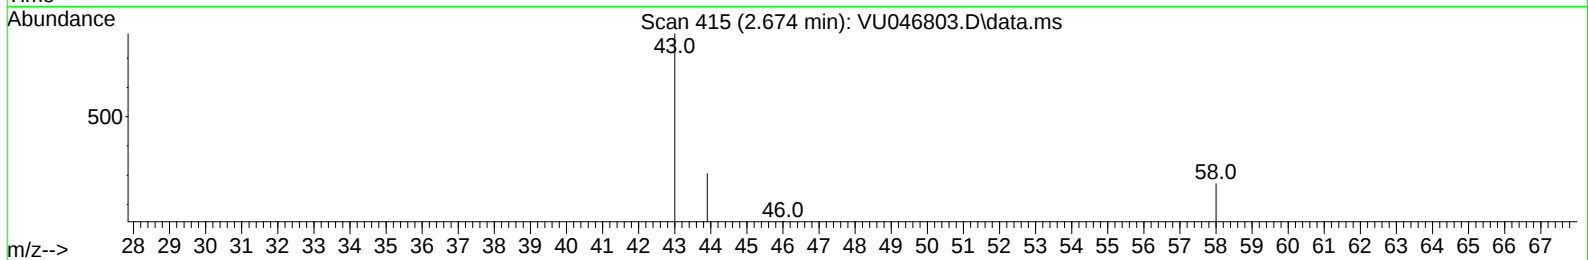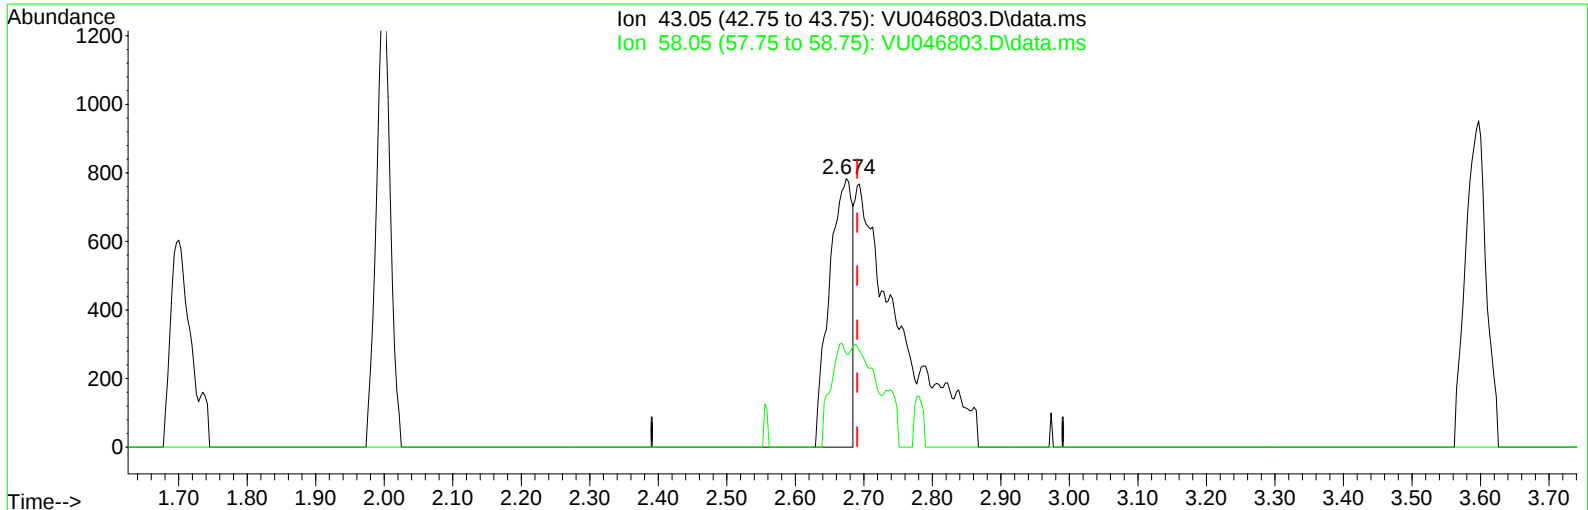

TIC: VU046803.D\data.ms

(13) Acetone (T)

2.674min (-0.016) 1.52 ug/L

response 1815

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	26.56
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012022\
 Data File : VU046803.D
 Acq On : 20 Jan 2022 11:40
 Operator : SY/MD
 Sample : VU0120WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK052

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/21/2022
 Supervised By :Mahesh Dadoda 01/21/2022

Quant Time: Jan 20 14:42:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 20 02:00:32 2022
 Response via : Initial Calibration

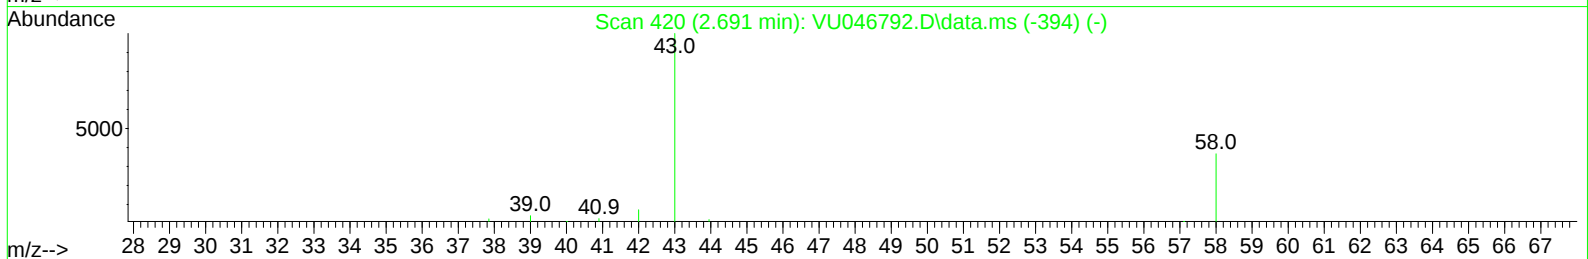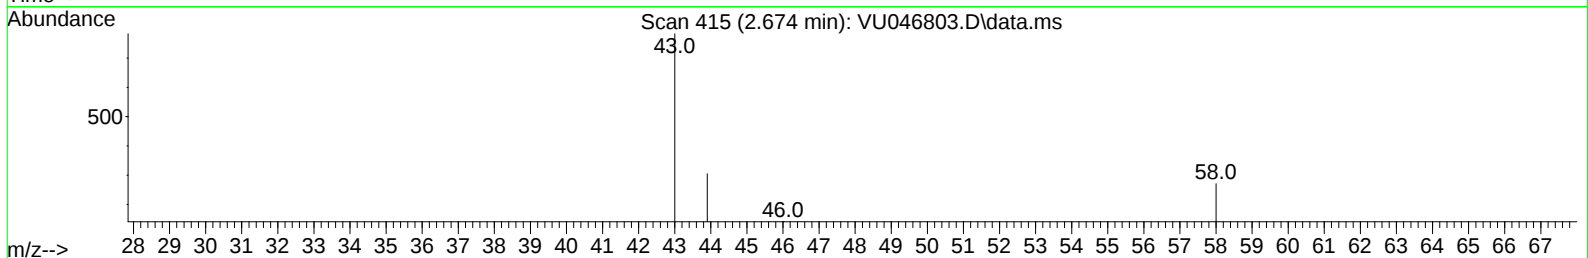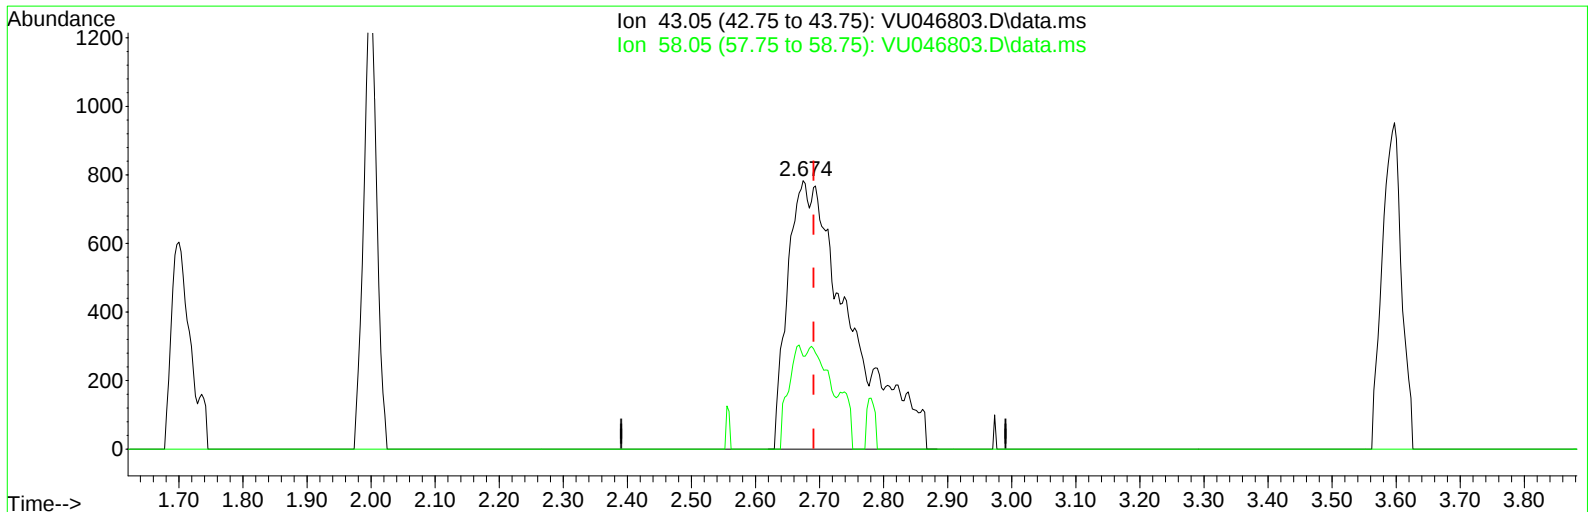

TIC: VU046803.D\data.ms

(13) Acetone (T)

2.674min (-0.016) 4.44 ug/L m

response 5304

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	9.09
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012022\
 Data File : VU046803.D
 Acq On : 20 Jan 2022 11:40
 Operator : SY/MD
 Sample : VU0120WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK052

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/21/2022
 Supervised By :Mahesh Dadoda 01/21/2022

Quant Time: Jan 20 14:42:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 20 02:00:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	87569	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	93881	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.815	152	46208	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	33501	4.515	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	90.200%	
7) Chloroethane-d5	1.919	69	29082	4.974	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	99.400%	
11) 1,1-Dichloroethene-d2	2.571	65	13930	4.719	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	94.400%	
20) 2-Butanone-d5	4.652	46	110608	50.316	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	100.640%	
24) Chloroform-d	5.066	84	63049	4.840	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.800%	
26) 1,2-Dichloroethane-d4	5.706	65	36937	5.207	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	104.200%	
32) Benzene-d6	5.729	84	129624	4.698	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.000%	
36) 1,2-Dichloropropane-d6	6.693	67	40077	4.838	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.800%	
41) Toluene-d8	7.899	98	108427	4.293	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.800%	
43) trans-1,3-Dichloroprop...	8.182	79	15834	4.352	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	87.000%	
46) 2-Hexanone-d5	8.639	63	99668	46.266	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	92.540%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	39674	4.770	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	95.400%	
66) 1,2-Dichlorobenzene-d4	12.195	152	42840	4.944	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	98.800%	
Target Compounds					Qvalue	
13) Acetone	2.674	43	5304m	4.436	ug/L	
38) Bromodichloromethane	7.111	83	1156	0.148	ug/L #	83
42) Toluene	7.973	91	10342	0.391	ug/L	93
49) Dibromochloromethane	8.812	129	348	0.064	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed