


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012022\
 Data File : VU046801.D
 Acq On : 20 Jan 2022 09:43
 Operator : SY/MD
 Sample : BFB045
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB045

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Jan 24 00:23:26 2022

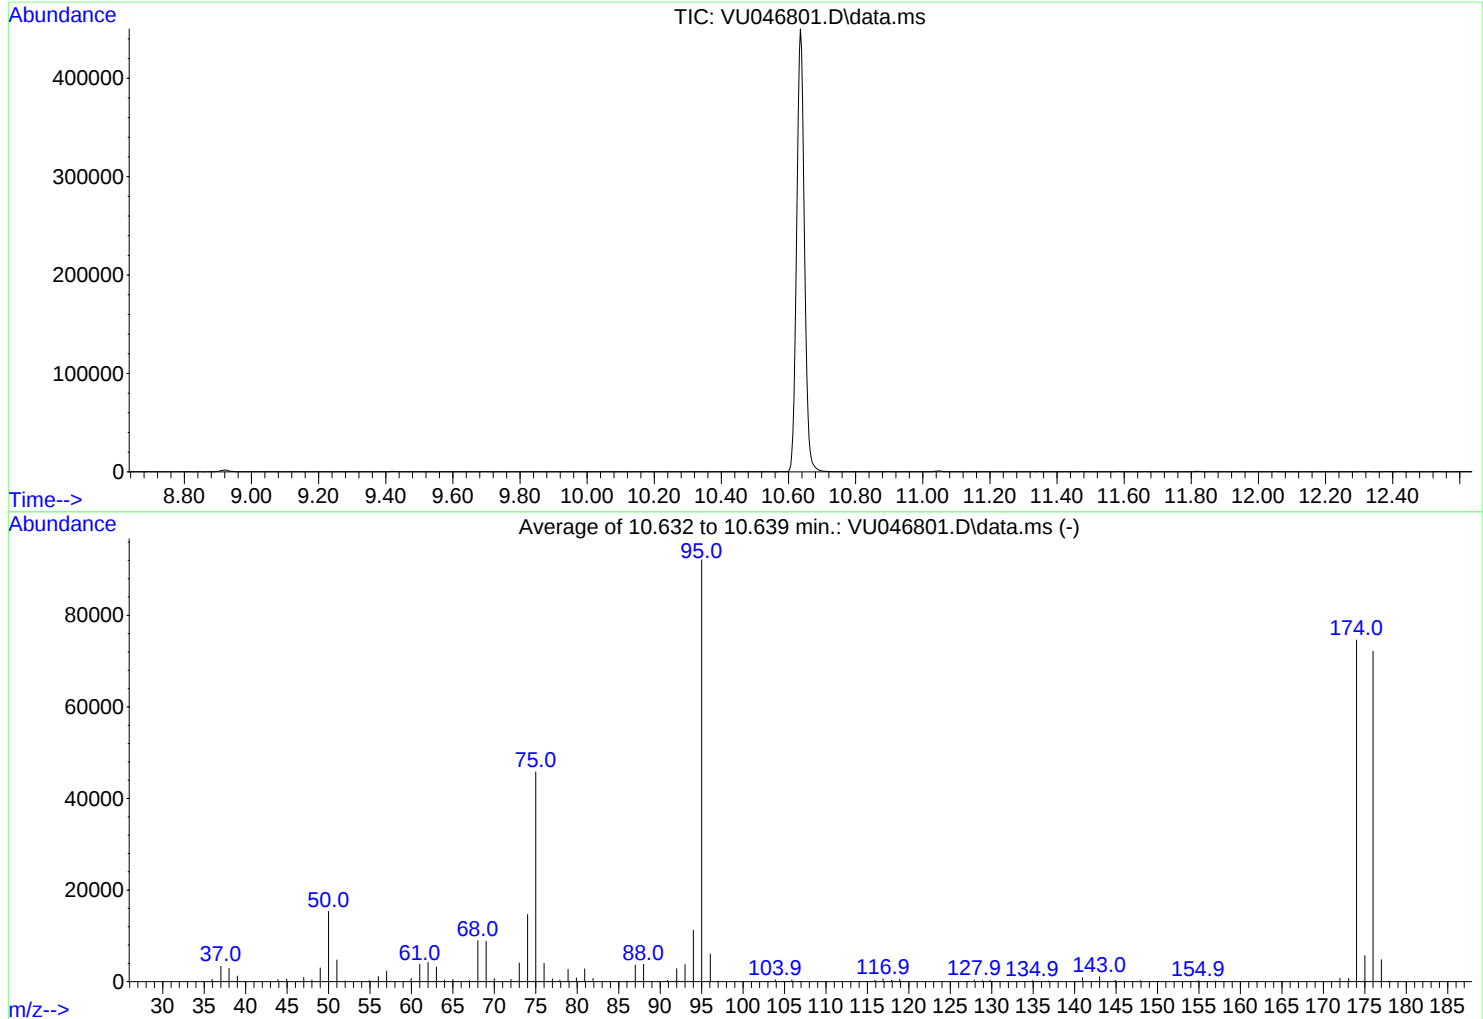

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	15342	PASS
75	95	30	80	49.7	45816	PASS
95	95	100	100	100.0	92128	PASS
96	95	5	9	6.6	6057	PASS
173	174	0.00	2	0.9	698	PASS
174	95	50	120	81.0	74611	PASS
175	174	5	9	7.6	5682	PASS
176	174	95	101	96.7	72160	PASS
177	176	5	9	6.7	4799	PASS

m/z	Abundance
36.00	531.0
37.00	3458.0
38.00	2995.0
39.00	1240.0
39.90	118.0
44.00	618.0
45.00	595.0
47.00	948.0
48.00	353.0
49.00	3064.0
50.00	15864.0
51.00	4855.0
52.00	187.0
54.90	253.0
56.00	1174.0
57.00	2347.0
60.00	695.0
61.00	3836.0
62.00	4386.0
63.00	3330.0
64.00	357.0
65.00	551.0
67.00	219.0
68.00	9226.0
69.00	9011.0
70.00	638.0
72.00	556.0
73.00	4229.0
74.00	15148.0
75.00	47248.0
76.00	4185.0
77.00	627.0
77.90	346.0
78.90	2788.0
79.90	830.0
80.90	2910.0
81.90	742.0
86.00	133.0
87.00	3719.0
88.00	3895.0
90.90	296.0
92.00	2928.0
93.00	3839.0
94.00	11617.0
95.00	95240.0
96.10	6231.0
97.00	163.0
103.90	396.0
104.80	118.0
105.90	378.0
106.80	116.0
112.90	112.0
115.90	308.0
116.90	645.0
117.90	334.0
118.90	553.0
127.90	370.0
128.90	221.0
129.80	337.0
134.90	214.0
136.90	141.0
140.90	856.0
143.00	1173.0
144.90	294.0
146.00	177.0
147.90	260.0
154.90	265.0
156.90	159.0
172.00	732.0
173.00	735.0
174.00	77096.0
175.00	5902.0
176.00	74504.0
177.00	4991.0
177.90	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045

m/z	Abundance
35.90	485.0
37.00	3352.0
38.00	2762.0
39.00	1156.0
39.90	113.0
44.00	542.0
44.90	564.0
47.00	860.0
48.00	372.0
49.00	2961.0
50.00	14750.0
51.00	4719.0
52.00	173.0
54.90	208.0
56.00	1164.0
57.00	2236.0
59.90	668.0
61.00	3644.0
62.00	3979.0
63.00	3163.0
64.00	332.0
65.00	524.0
67.00	209.0
68.00	8889.0
69.00	8552.0
70.00	596.0
72.00	551.0
73.00	3996.0
74.00	14209.0
75.00	44704.0
76.00	3753.0
77.00	551.0
77.90	364.0
78.90	2662.0
79.90	725.0
80.90	2792.0
81.90	668.0
86.00	120.0
87.00	3695.0
88.00	3591.0
90.90	305.0
92.00	2771.0
93.00	3649.0
94.00	10935.0
95.00	91024.0
96.00	5974.0
97.00	157.0
103.90	377.0
105.90	364.0
106.90	111.0
112.90	100.0
115.90	332.0
116.90	562.0
117.90	323.0
118.90	536.0
127.90	386.0
128.90	210.0
129.80	361.0
134.90	193.0
136.90	145.0
140.90	866.0
143.00	1116.0
144.90	220.0
146.00	141.0
147.90	253.0
154.90	247.0
157.00	180.0
172.00	647.0
173.10	700.0
174.00	75592.0
175.00	5592.0
176.00	72424.0
177.00	4598.0
177.90	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045

m/z	Abundance
43.90	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045

m/z	Abundance
36.00	536.0
37.00	3285.0
38.00	2969.0
39.00	1259.0
39.90	121.0
43.90	632.0
44.90	637.0
47.00	948.0
48.00	392.0
49.00	3034.0
50.00	15411.0
51.00	4579.0
52.00	193.0
54.90	245.0
56.00	1081.0
57.00	2324.0
60.00	687.0
61.00	3799.0
62.00	4238.0
63.00	3182.0
64.00	375.0
65.00	506.0
67.00	185.0
68.00	8766.0
69.00	8890.0
70.00	639.0
72.00	489.0
73.00	3982.0
74.00	14555.0
75.00	45496.0
76.00	4071.0
77.00	592.0
77.90	307.0
78.90	2637.0
79.90	850.0
80.90	2737.0
81.90	708.0
85.90	146.0
87.00	3547.0
88.00	3794.0
90.90	258.0
92.00	2782.0
93.00	3755.0
94.00	11151.0
95.00	90120.0
96.10	5965.0
97.00	136.0
103.90	393.0
104.90	122.0
105.90	374.0
114.90	107.0
115.90	273.0
116.90	680.0
117.90	291.0
118.90	521.0
127.90	300.0
128.90	194.0
129.80	281.0
134.90	218.0
136.80	143.0
141.00	771.0
143.00	1127.0
144.90	308.0
146.00	142.0
147.90	230.0
154.90	262.0
156.90	130.0
172.00	743.0
173.00	658.0
174.00	71144.0
175.00	5552.0
176.00	69552.0
177.00	4808.0
177.90	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB045