

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
 Data File : VU057652.D
 Acq On : 25 Jan 2024 05:01
 Operator : MD/SY
 Sample : P1229-34 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jan 25 05:45:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 25 04:41:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	53151	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	47318	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	21775	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	13069	4.463	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.200%
7) Chloroethane-d5	1.914	69	11309	4.609	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.200%
11) 1,1-Dichloroethene-d2	2.563	65	6136	4.456	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	89.200%
20) 2-Butanone-d5	4.653	46	33904	61.370	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	122.740%
24) Chloroform-d	5.055	84	30206	5.082	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.600%
26) 1,2-Dichloroethane-d4	5.695	65	15028	5.563	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.200%
32) Benzene-d6	5.721	84	57408	5.172	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.400%
36) 1,2-Dichloropropane-d6	6.685	67	18238	5.448	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.000%
41) Toluene-d8	7.894	98	50480	4.791	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.800%
43) trans-1,3-Dichloroprop...	8.177	79	6566	4.921	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.400%
46) 2-Hexanone-d5	8.634	63	24612	57.815	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	115.620%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	12511	5.575	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	111.600%
66) 1,2-Dichlorobenzene-d4	12.190	152	16682	5.459	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.200%
Target Compounds						
16) Methylene chloride	3.042	84	1701	0.410	ug/L	92
35) Methylcyclohexane	6.685	83	4164	0.576	ug/L #	18
37) 1,2-Dichloropropane	6.682	63	2048	0.504	ug/L #	89
61) 1,2,3-Trichloropropane	11.807	75	2564	1.173	ug/L #	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
Data File : VU057652.D
Acq On : 25 Jan 2024 05:01
Operator : MD/SY
Sample : P1229-34 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Jan 25 05:45:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 25 04:41:48 2024
Response via : Initial Calibration

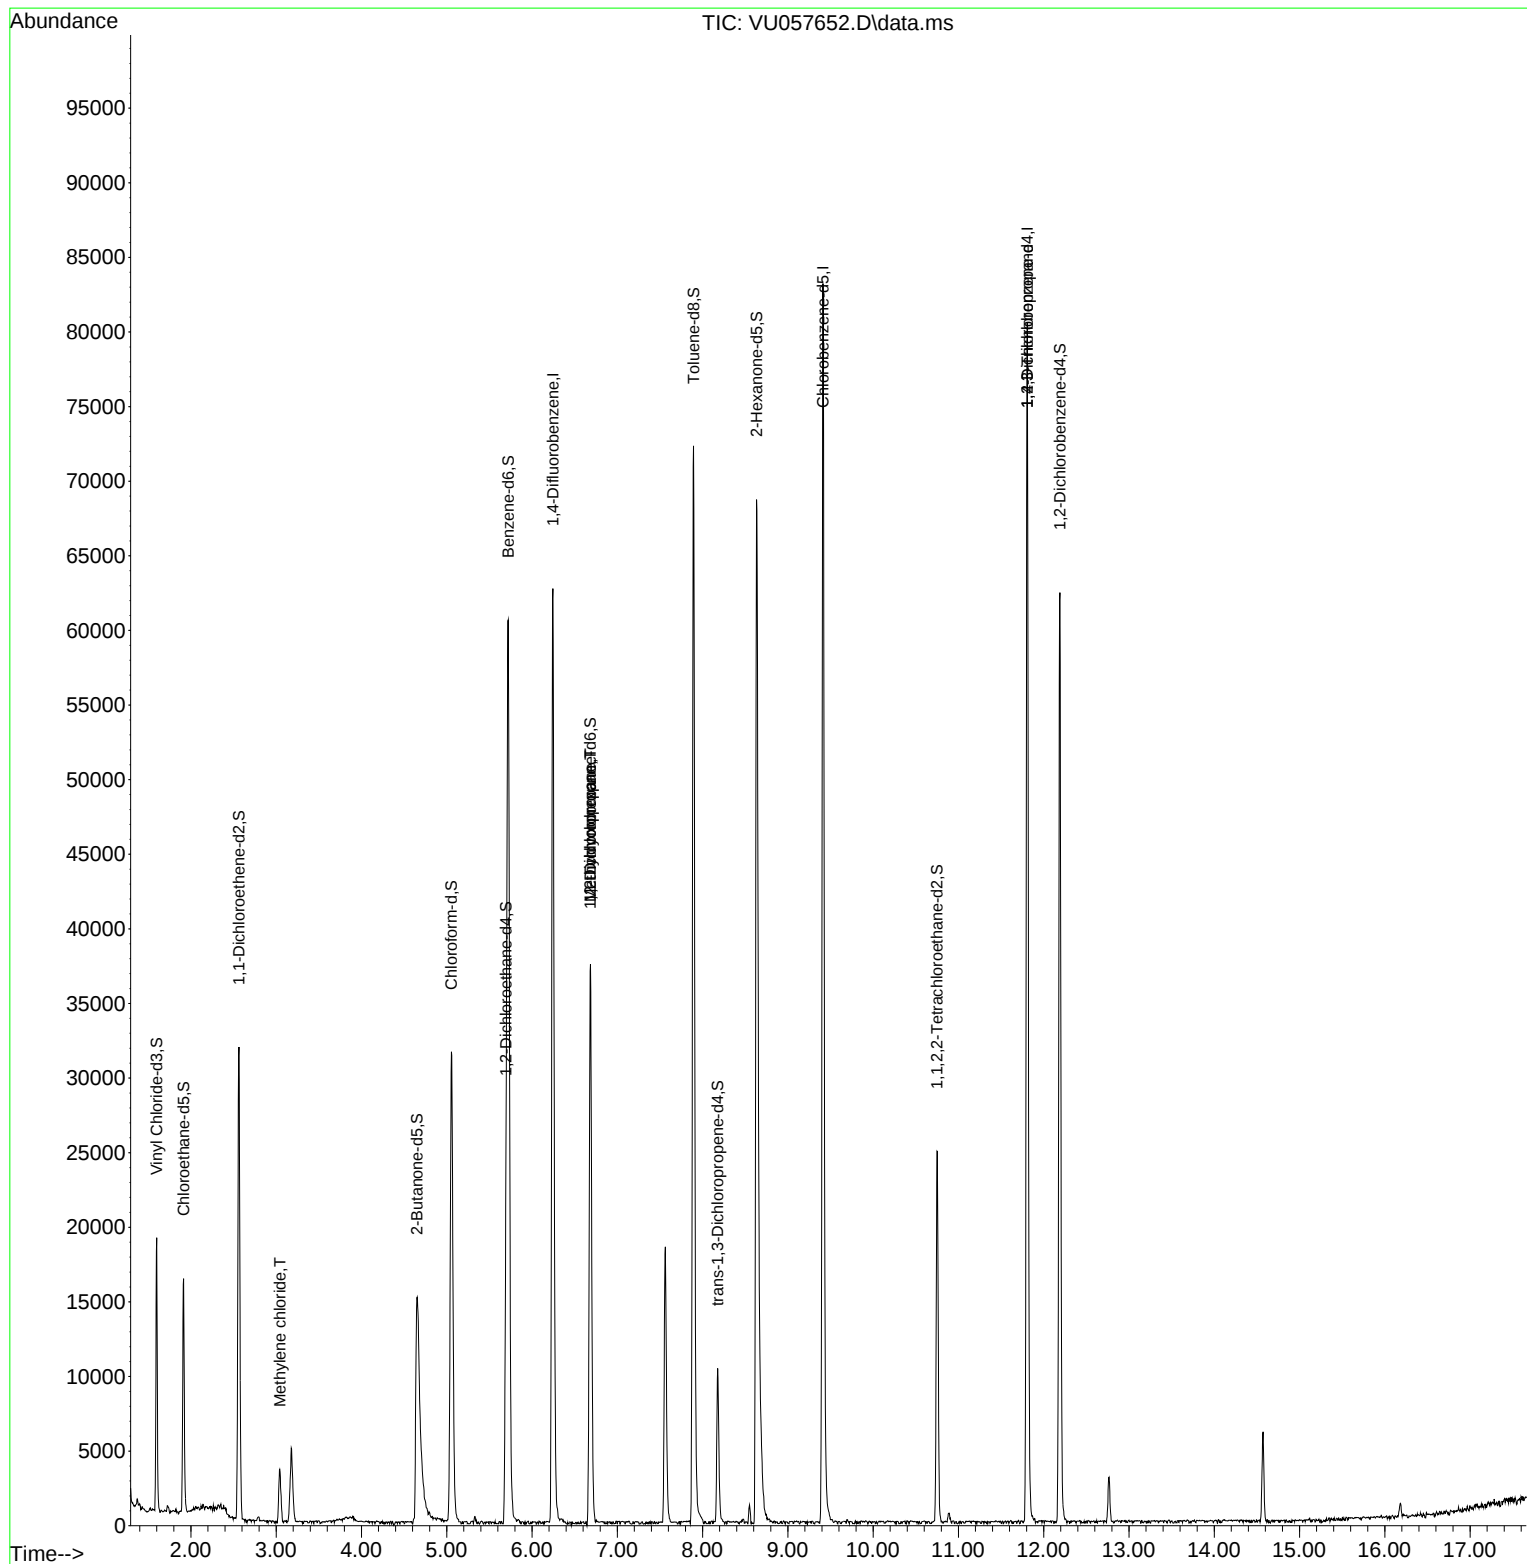



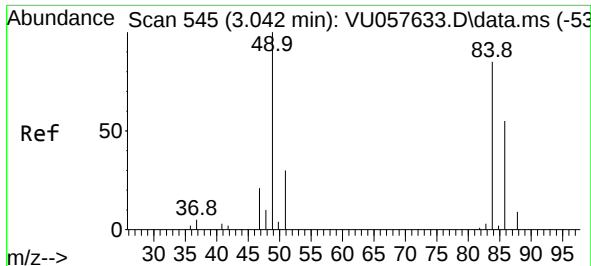


#16
Methylene chloride
Concen: 0.410 ug/L
RT: 3.042 min Scan# 54
Delta R.T. -0.000 min
Lab File: VU057652.D
Acq: 25 Jan 2024 05:01

Instrument :
MSVOA_U
ClientSampleId :



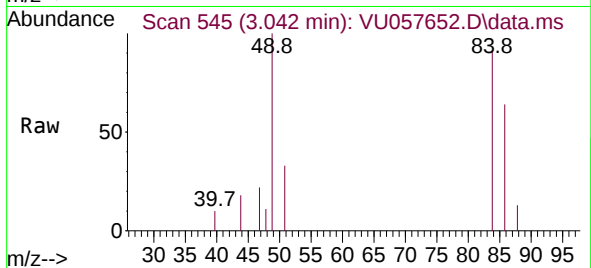



Tgt Ion: 84 Resp: 1701
Ion Ratio Lower Upper
84 100
86 70.4 43.5 80.9
49 110.2 82.5 153.1

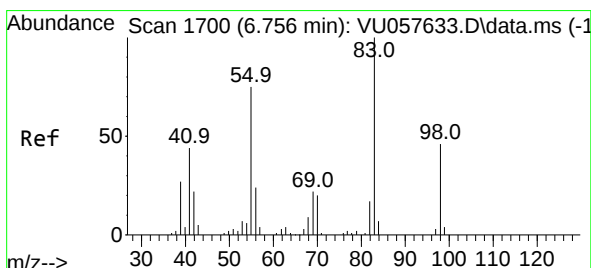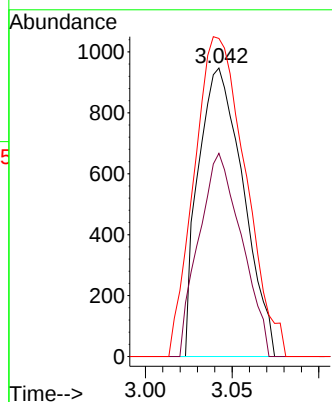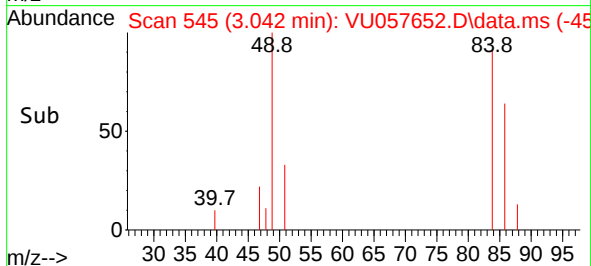

#35
Methylcyclohexane
Concen: 0.576 ug/L
RT: 6.685 min Scan# 1678
Delta R.T. -0.071 min
Lab File: VU057652.D
Acq: 25 Jan 2024 05:01

Tgt Ion: 83 Resp: 4164
Ion Ratio Lower Upper
83 100
55 0.0 61.4 92.0#
98 0.0 38.2 57.4#

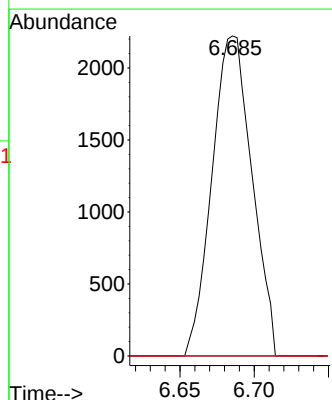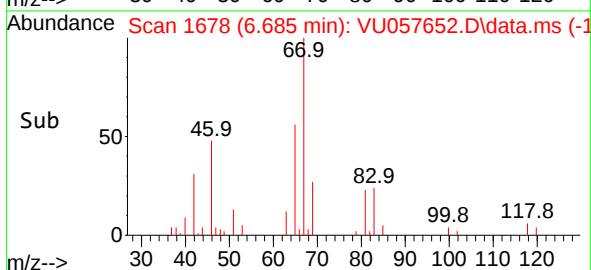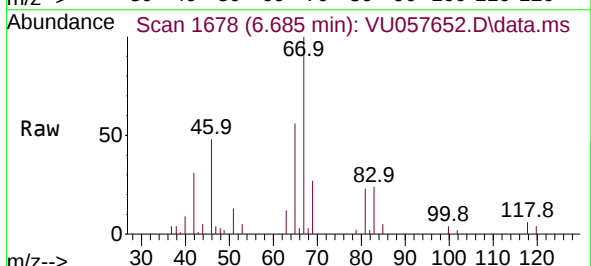

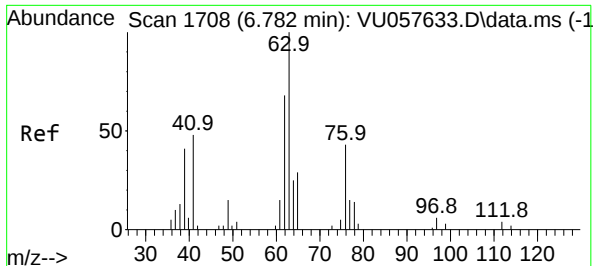

#37

1,2-Dichloropropane

Concen: 0.504 ug/L

RT: 6.682 min Scan# 1

Delta R.T. -0.100 min

Lab File: VU057652.D

Acq: 25 Jan 2024 05:01

Instrument :

MSVOA_U





ClientSampleId :

Tgt Ion: 63 Resp: 2048

Ion Ratio Lower Upper

63 100

112 0.0 3.0 4.4#

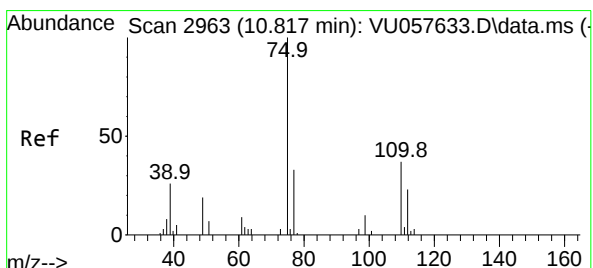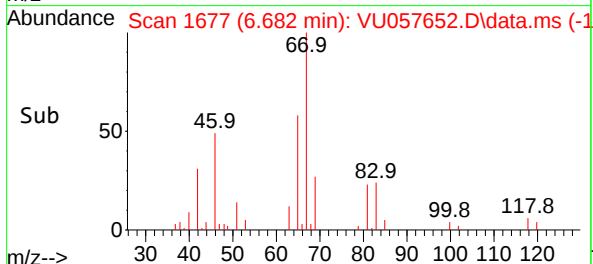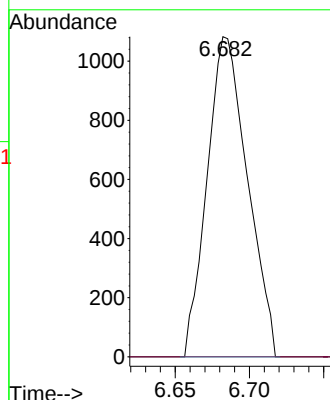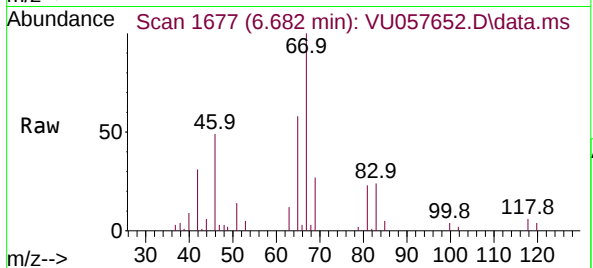

#61

1,2,3-Trichloropropane

Concen: 1.173 ug/L

RT: 11.807 min Scan# 3271

Delta R.T. 0.990 min

Lab File: VU057652.D

Acq: 25 Jan 2024 05:01

Tgt Ion: 75 Resp: 2564

Ion Ratio Lower Upper

75 100

110 0.0 30.1 45.1#

77 36.7 25.5 38.3

