

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
 Data File : VU057638.D
 Acq On : 24 Jan 2024 23:23
 Operator : MD/SY
 Sample : P1227-11DL 400X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B87DL

Quant Time: Jan 25 04:58:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 25 04:41:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	58795	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	53266	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	25089	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	13862	4.279	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.600%
7) Chloroethane-d5	1.914	69	11844	4.363	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.200%
11) 1,1-Dichloroethene-d2	2.563	65	6587	4.324	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.400%
20) 2-Butanone-d5	4.640	46	31683	51.844	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.680%
24) Chloroform-d	5.055	84	30429	4.628	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.600%
26) 1,2-Dichloroethane-d4	5.695	65	15106	5.056	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.200%
32) Benzene-d6	5.721	84	59774	4.784	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%
36) 1,2-Dichloropropane-d6	6.685	67	18867	5.006	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.200%
41) Toluene-d8	7.894	98	55347	4.666	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.400%
43) trans-1,3-Dichloroprop...	8.177	79	6619	4.407	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.200%
46) 2-Hexanone-d5	8.631	63	24664	51.467	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.940%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	12387	4.904	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.000%
66) 1,2-Dichlorobenzene-d4	12.190	152	17862	5.073	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.400%
Target Compounds						Qvalue
16) Methylene chloride	3.046	84	949	0.207	ug/L	98
47) Tetrachloroethene	8.547	164	29881	8.073	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
Data File : VU057638.D
Acq On : 24 Jan 2024 23:23
Operator : MD/SY
Sample : P1227-11DL 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B87DL

Quant Time: Jan 25 04:58:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 25 04:41:48 2024
Response via : Initial Calibration




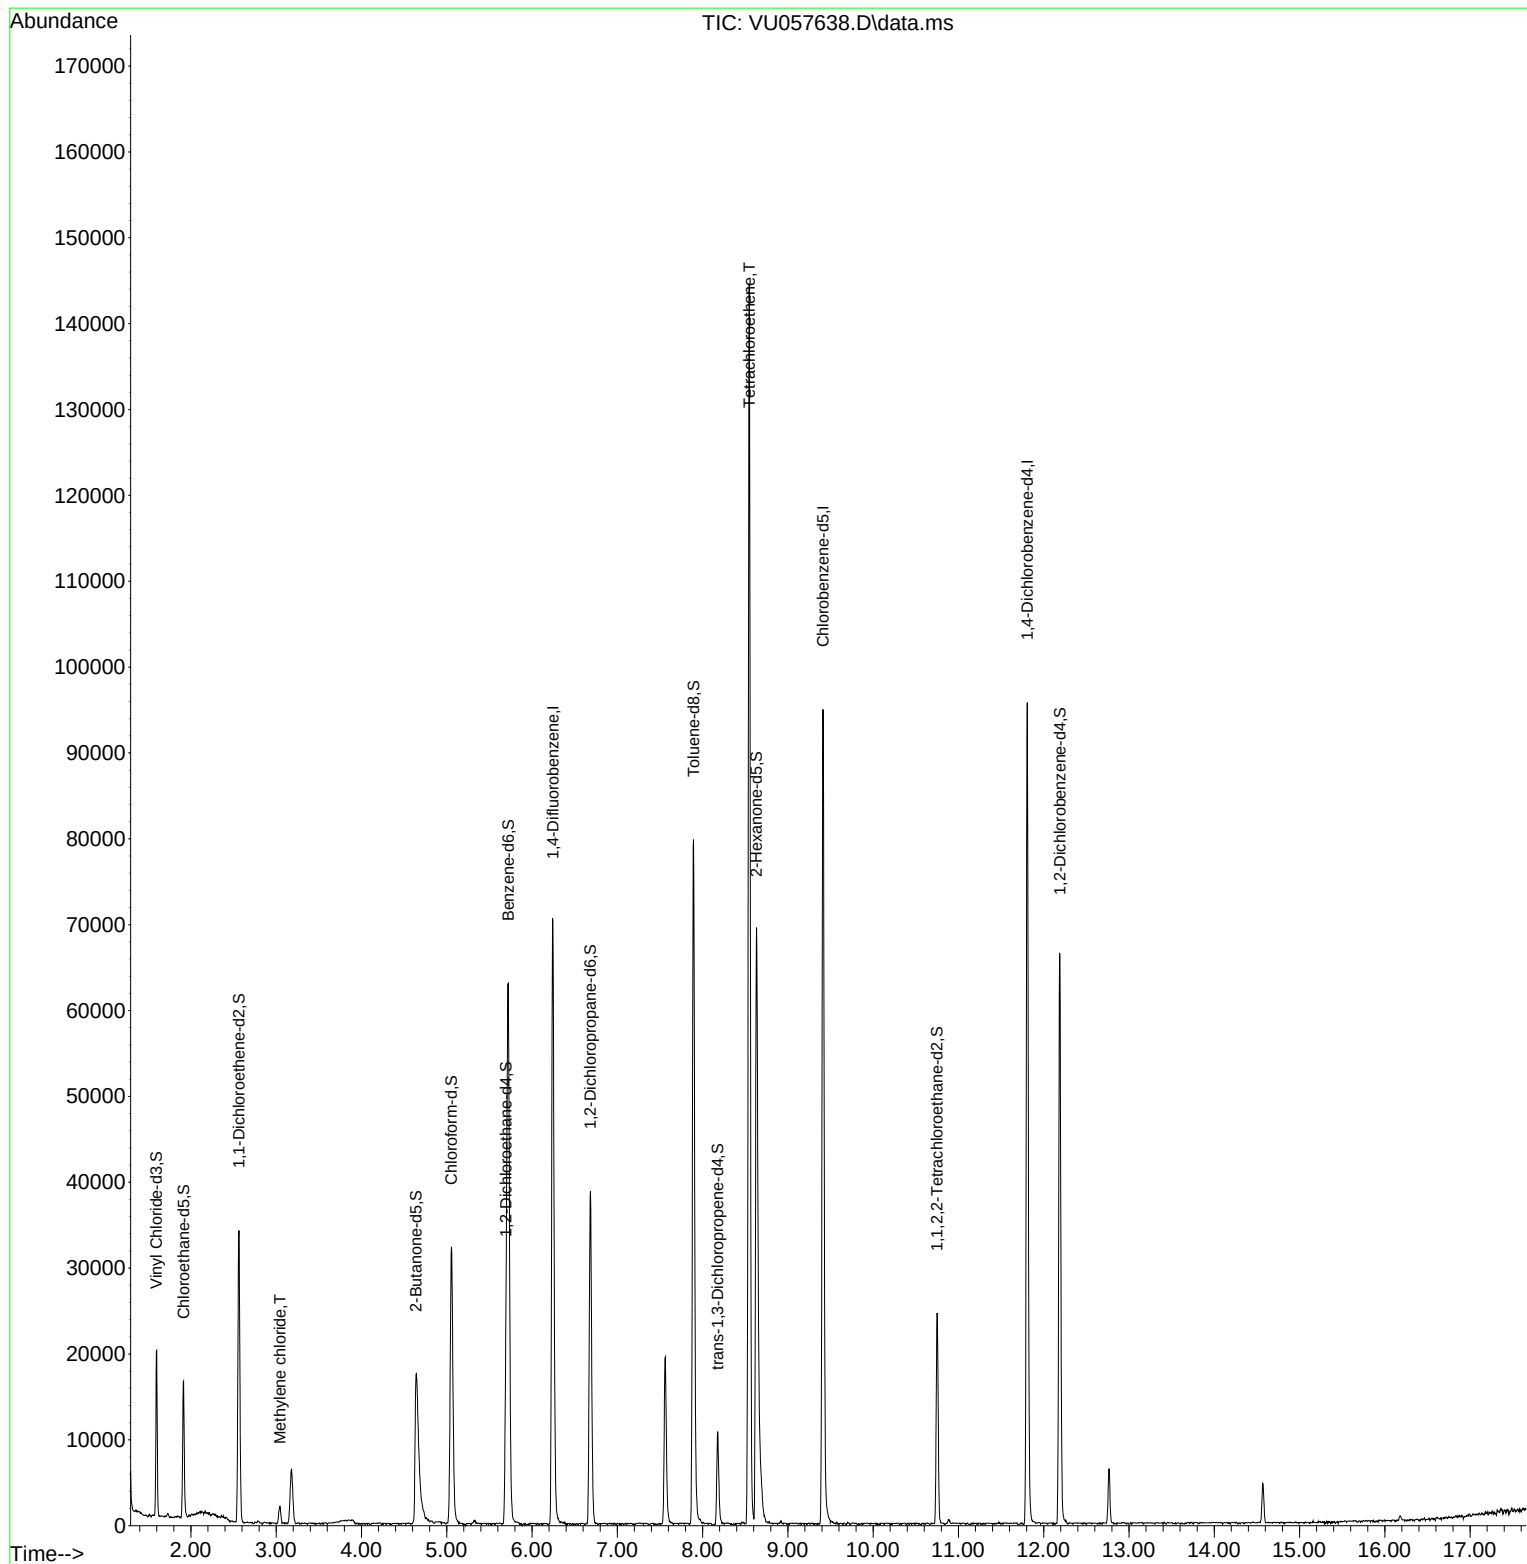


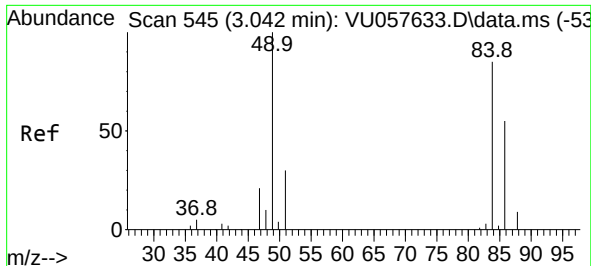

#16
Methylene chloride
Concen: 0.207 ug/L
RT: 3.046 min Scan# 54
Delta R.T. 0.003 min
Lab File: VU057638.D
Acq: 24 Jan 2024 23:23

Instrument :
MSVOA_U
ClientSampleId :
C0B87DL

Tgt Ion: 84 Resp: 949
Ion Ratio Lower Upper
84 100
86 62.8 43.5 80.9
49 120.0 82.5 153.1

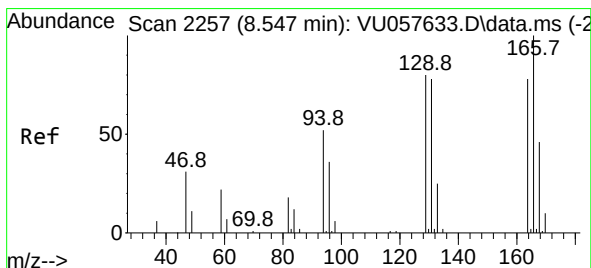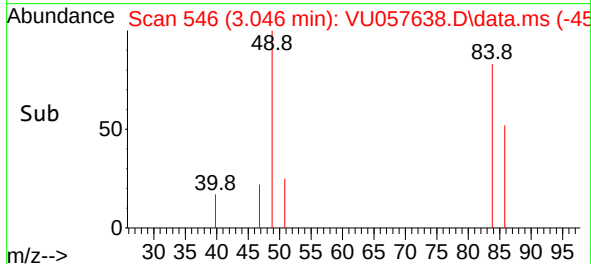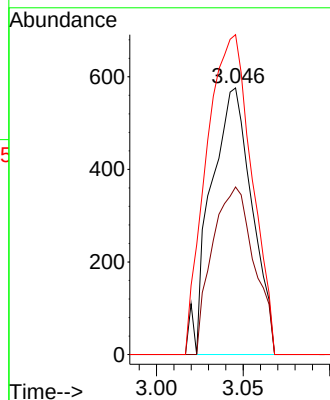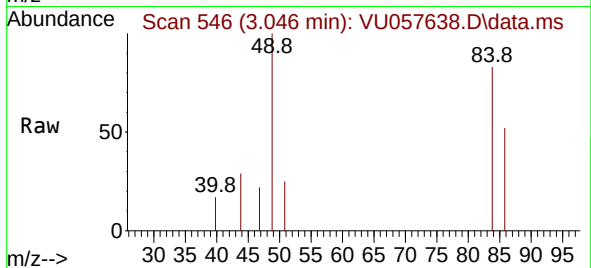

#47
Tetrachloroethene
Concen: 8.073 ug/L
RT: 8.547 min Scan# 2257
Delta R.T. -0.000 min
Lab File: VU057638.D
Acq: 24 Jan 2024 23:23

Tgt Ion: 164 Resp: 29881
Ion Ratio Lower Upper
164 100
129 103.6 71.3 132.5
131 98.8 68.1 126.5
166 131.0 87.4 162.4

