

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
 Data File : VU057632.D
 Acq On : 24 Jan 2024 20:34
 Operator : MD/SY
 Sample : P1227-06DL 400X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B82DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057632.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	108	rVB	19703	22718	9.77%	1.360%
2	1.914	185	194	203	rBV	16441	21806	9.38%	1.305%
3	2.563	385	396	411	rVB	34894	56329	24.22%	3.371%
4	3.042	537	545	554	rVB2	1850	3082	1.33%	0.184%
5	3.181	575	588	604	rBV	7583	17041	7.33%	1.020%
6	4.644	1031	1043	1081	rBV	17950	56324	24.22%	3.371%
7	5.055	1158	1171	1196	rVB	32320	73064	31.41%	4.373%
8	5.718	1360	1377	1403	rBV2	64406	161732	69.54%	9.679%
9	6.245	1529	1541	1562	rBV	68192	130798	56.24%	7.828%
10	6.685	1665	1678	1699	rVB	39053	74997	32.25%	4.488%
11	7.563	1940	1951	1971	rBV2	19826	34982	15.04%	2.094%
12	7.894	2042	2054	2073	rBV	78234	139798	60.11%	8.366%
13	8.177	2131	2142	2161	rBV2	10687	19320	8.31%	1.156%
14	8.547	2245	2257	2274	rBV	138153	232577	100.00%	13.919%
15	8.634	2274	2284	2321	rVB2	70878	152190	65.44%	9.108%
16	9.412	2514	2526	2552	rBV	89481	155742	66.96%	9.321%
17	10.750	2931	2942	2956	rVB	24866	39545	17.00%	2.367%
18	11.807	3260	3271	3291	rBV	90187	148213	63.73%	8.870%
19	12.187	3376	3389	3410	rBV	66984	111537	47.96%	6.675%
20	12.766	3559	3569	3581	rVB2	9556	14650	6.30%	0.877%
21	14.573	4120	4131	4139	rBV	2927	4502	1.94%	0.269%




Sum of corrected areas: 1670947

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
Data File : VU057632.D
Acq On : 24 Jan 2024 20:34
Operator : MD/SY
Sample : P1227-06DL 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B82DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

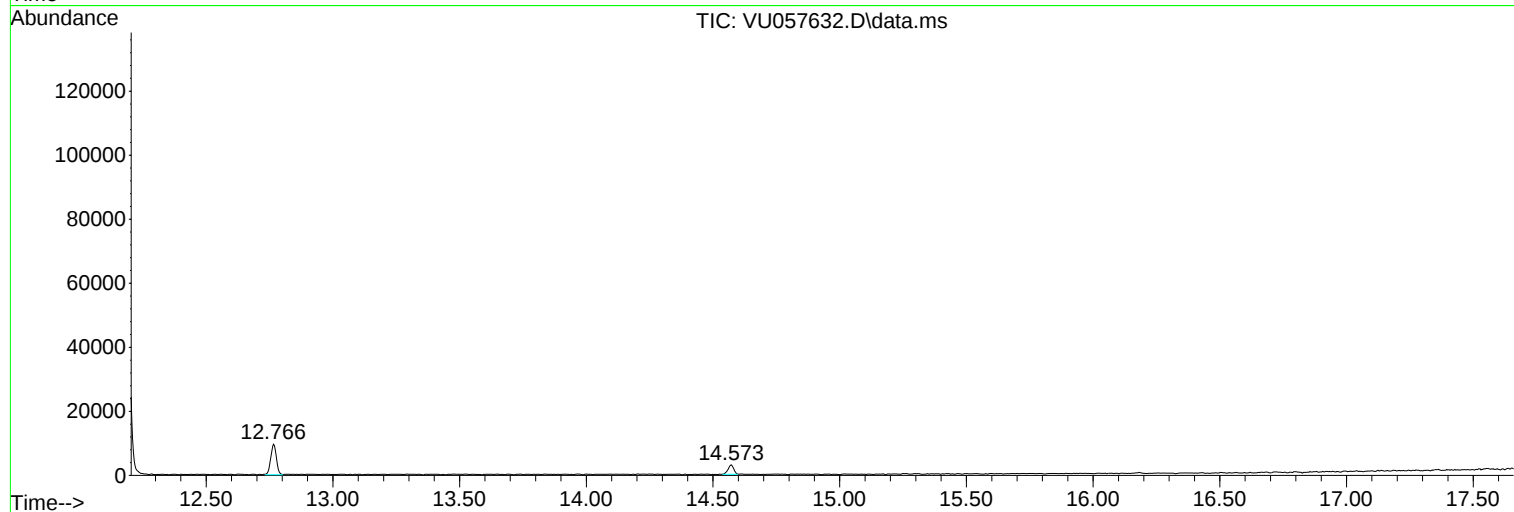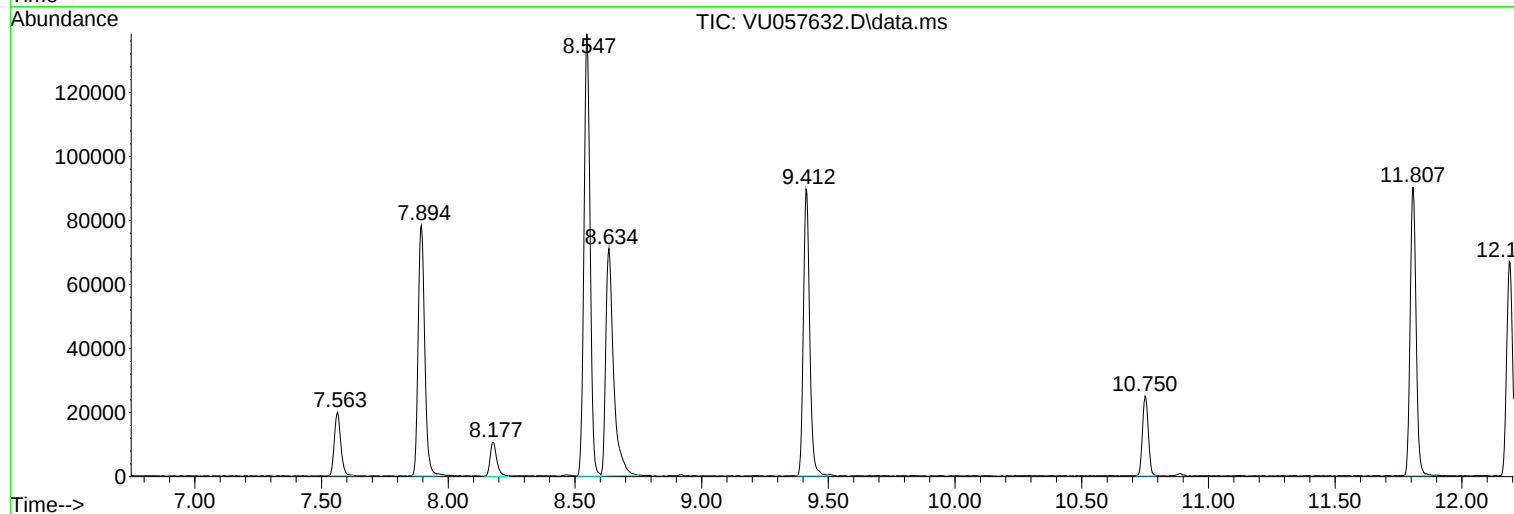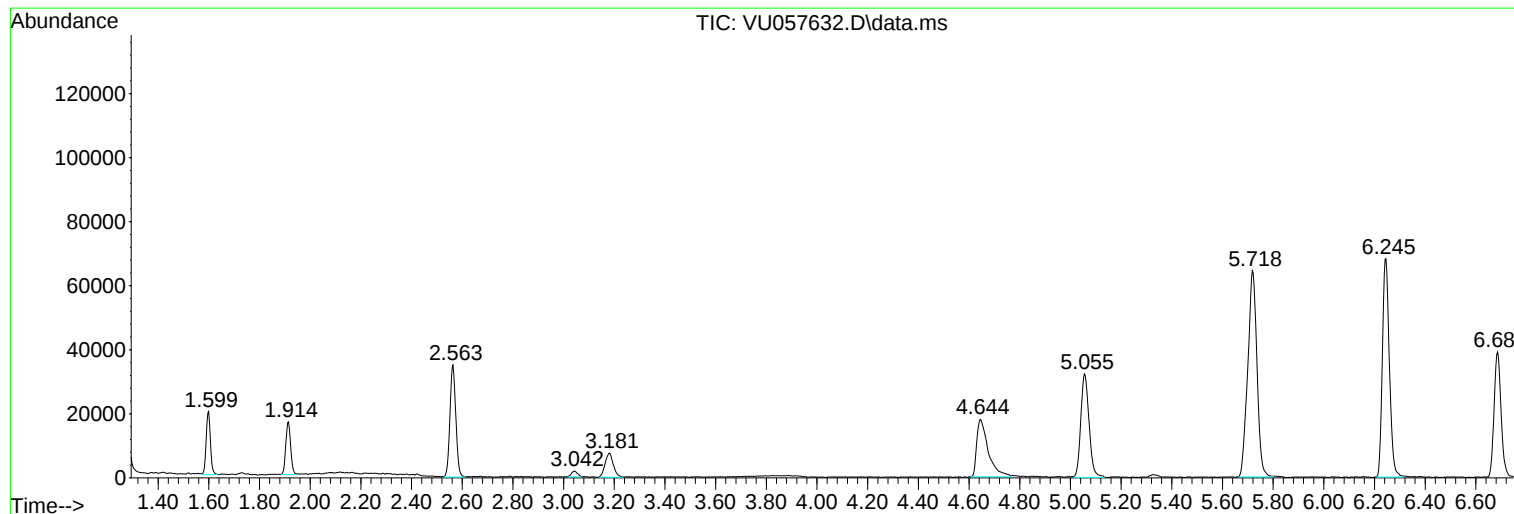

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
Data File : VU057632.D
Acq On : 24 Jan 2024 20:34
Operator : MD/SY
Sample : P1227-06DL 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B82DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
Data File : VU057632.D
Acq On : 24 Jan 2024 20:34
Operator : MD/SY
Sample : P1227-06DL 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B82DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------