

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
 Data File : VU057636.D
 Acq On : 24 Jan 2024 22:34
 Operator : MD/SY
 Sample : P1227-09DL 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B85DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057636.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	87	96	110	rVB	19671	22464	9.50%	1.328%
2	1.914	185	194	206	rBV	16395	21671	9.16%	1.282%
3	2.563	385	396	413	rVB	34237	54396	23.00%	3.217%
4	3.042	537	545	559	rVB3	2458	4545	1.92%	0.269%
5	3.177	573	587	607	rVB2	10588	24569	10.39%	1.453%
6	4.644	1030	1043	1084	rBV	18889	60355	25.52%	3.569%
7	5.055	1157	1171	1192	rBV	33052	72855	30.81%	4.309%
8	5.717	1356	1377	1399	rBV2	64716	164924	69.74%	9.753%
9	6.245	1529	1541	1570	rBV	69167	132892	56.19%	7.859%
10	6.685	1666	1678	1693	rBV	39393	76405	32.31%	4.518%
11	7.563	1938	1951	1966	rBV2	19568	36046	15.24%	2.132%
12	7.894	2041	2054	2080	rBV	78791	139670	59.06%	8.260%
13	8.177	2132	2142	2158	rBV2	10735	18715	7.91%	1.107%
14	8.547	2246	2257	2274	rBV	140735	236485	100.00%	13.985%
15	8.634	2274	2284	2320	rVB3	72776	157925	66.78%	9.339%
16	9.412	2515	2526	2547	rBV	90557	155644	65.82%	9.205%
17	10.749	2931	2942	2957	rVB	25655	42007	17.76%	2.484%
18	11.807	3260	3271	3294	rVB	91569	146947	62.14%	8.690%
19	12.190	3379	3390	3410	rBV	68000	110640	46.79%	6.543%
20	12.765	3561	3569	3578	rBV3	2232	3473	1.47%	0.205%
21	14.569	4121	4130	4144	rVB	5353	8311	3.51%	0.492%




Sum of corrected areas: 1690939

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
Data File : VU057636.D
Acq On : 24 Jan 2024 22:34
Operator : MD/SY
Sample : P1227-09DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B85DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

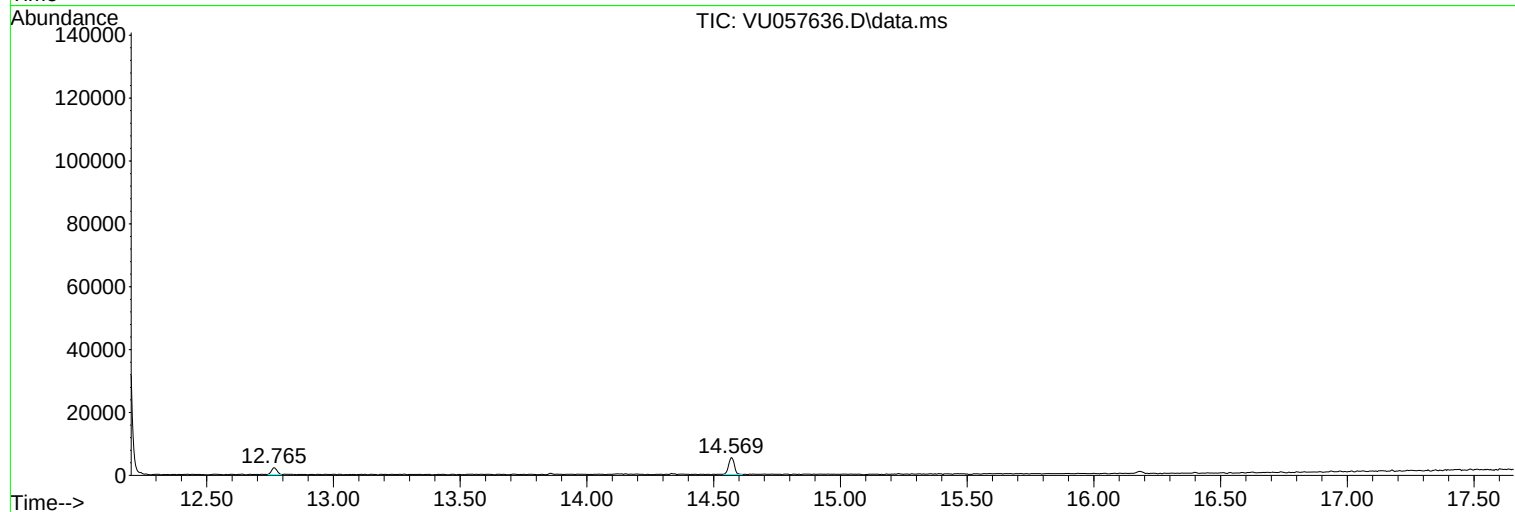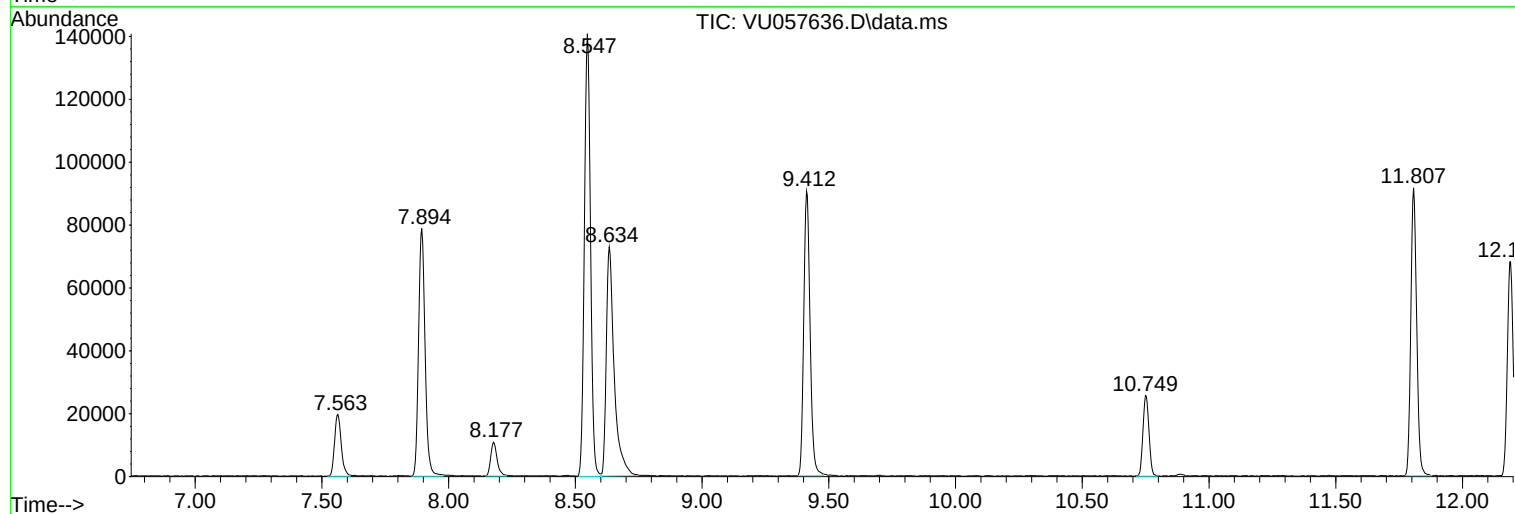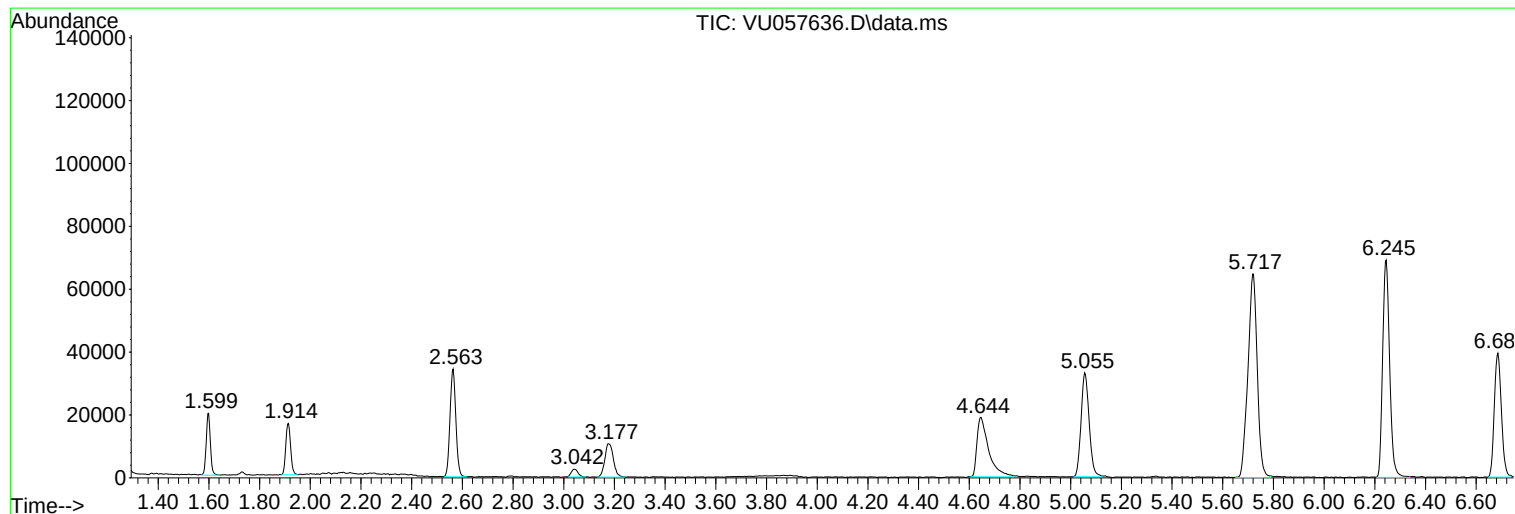

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
Data File : VU057636.D
Acq On : 24 Jan 2024 22:34
Operator : MD/SY
Sample : P1227-09DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B85DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
Data File : VU057636.D
Acq On : 24 Jan 2024 22:34
Operator : MD/SY
Sample : P1227-09DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B85DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc