

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
 Data File : VU057638.D
 Acq On : 24 Jan 2024 23:23
 Operator : MD/SY
 Sample : P1227-11DL 400X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B87DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057638.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	104	rVB	19277	21792	9.01%	1.297%
2	1.914	185	194	209	rBV	15832	21430	8.87%	1.276%
3	2.563	385	396	412	rVB	33988	54875	22.70%	3.267%
4	3.046	537	546	553	rVB3	1982	3303	1.37%	0.197%
5	3.181	574	588	604	rBV	6359	14118	5.84%	0.841%
6	4.644	1028	1043	1076	rBV	17454	54684	22.62%	3.256%
7	5.055	1157	1171	1193	rBV	32140	71451	29.56%	4.254%
8	5.721	1360	1378	1403	rBV2	62899	160798	66.52%	9.574%
9	6.242	1528	1540	1567	rBV	70560	135533	56.07%	8.070%
10	6.685	1666	1678	1695	rBV	38705	75045	31.04%	4.468%
11	7.563	1939	1951	1966	rBV	19387	34156	14.13%	2.034%
12	7.894	2041	2054	2077	rBV	79655	140788	58.24%	8.382%
13	8.177	2133	2142	2158	rBV	10792	18442	7.63%	1.098%
14	8.547	2245	2257	2274	rBV	144457	241733	100.00%	14.393%
15	8.634	2274	2284	2311	rVV3	68949	146603	60.65%	8.729%
16	9.412	2515	2526	2553	rBV	94819	162893	67.39%	9.699%
17	10.750	2932	2942	2956	rBV	24510	39679	16.41%	2.362%
18	11.807	3258	3271	3289	rBV	95717	154230	63.80%	9.183%
19	12.187	3378	3389	3410	rBV	66462	111126	45.97%	6.616%
20	12.766	3560	3569	3579	rBV2	6348	9539	3.95%	0.568%
21	14.569	4121	4130	4140	rVB	4580	7340	3.04%	0.437%




Sum of corrected areas: 1679558

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
Data File : VU057638.D
Acq On : 24 Jan 2024 23:23
Operator : MD/SY
Sample : P1227-11DL 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B87DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

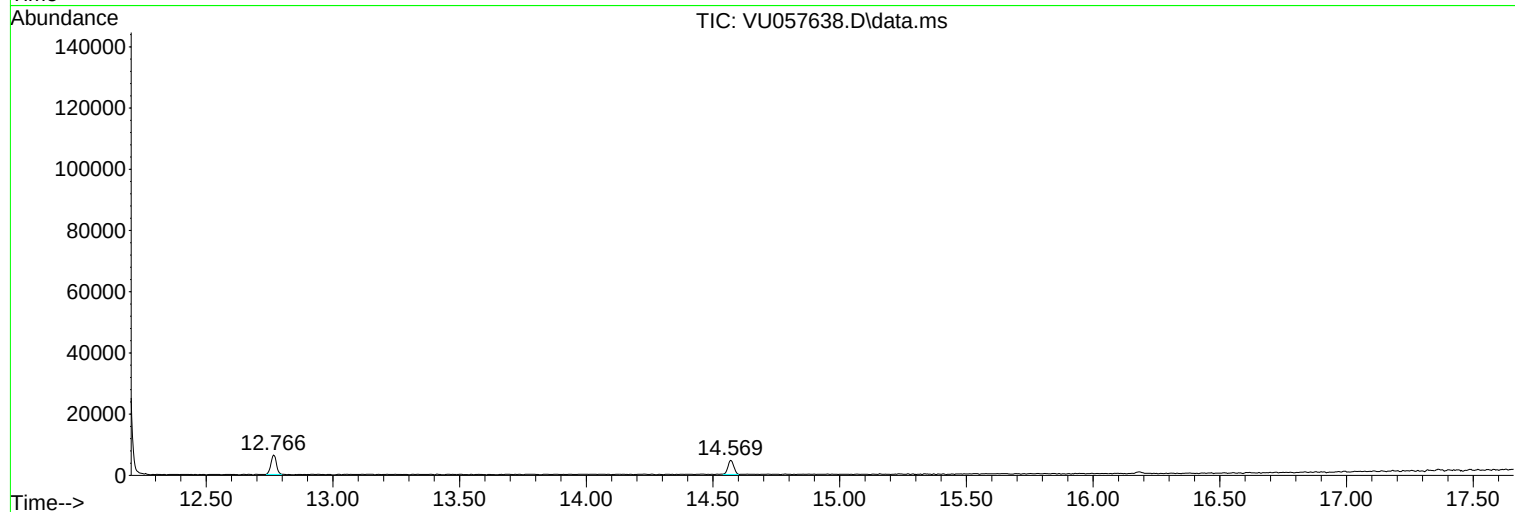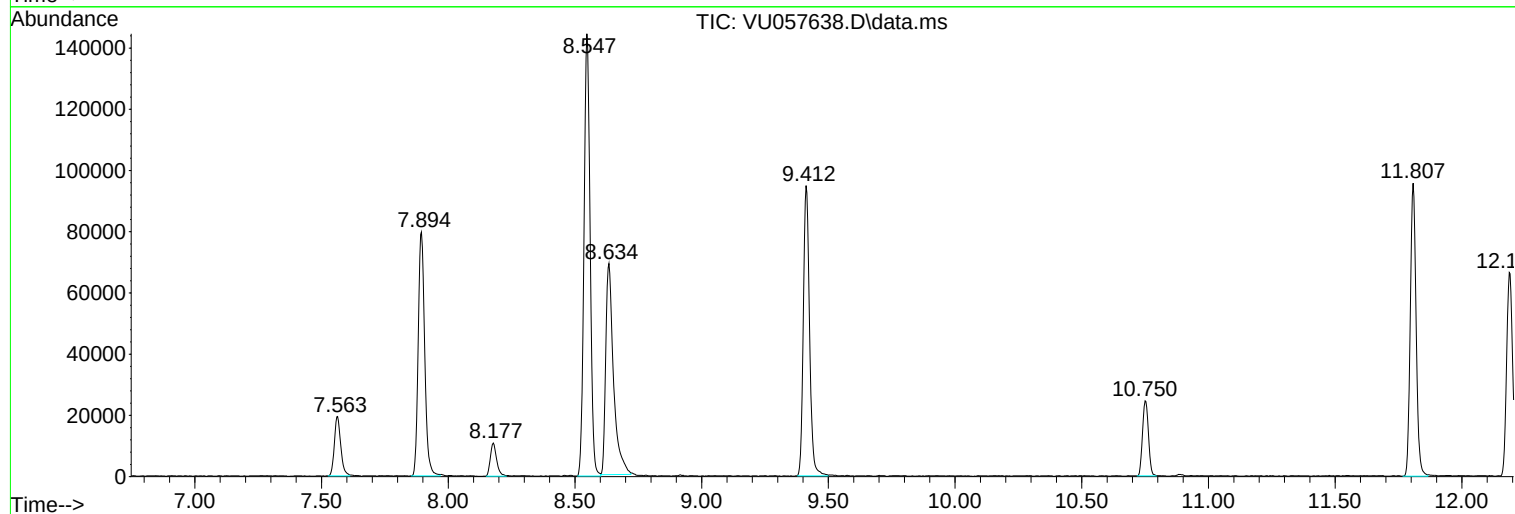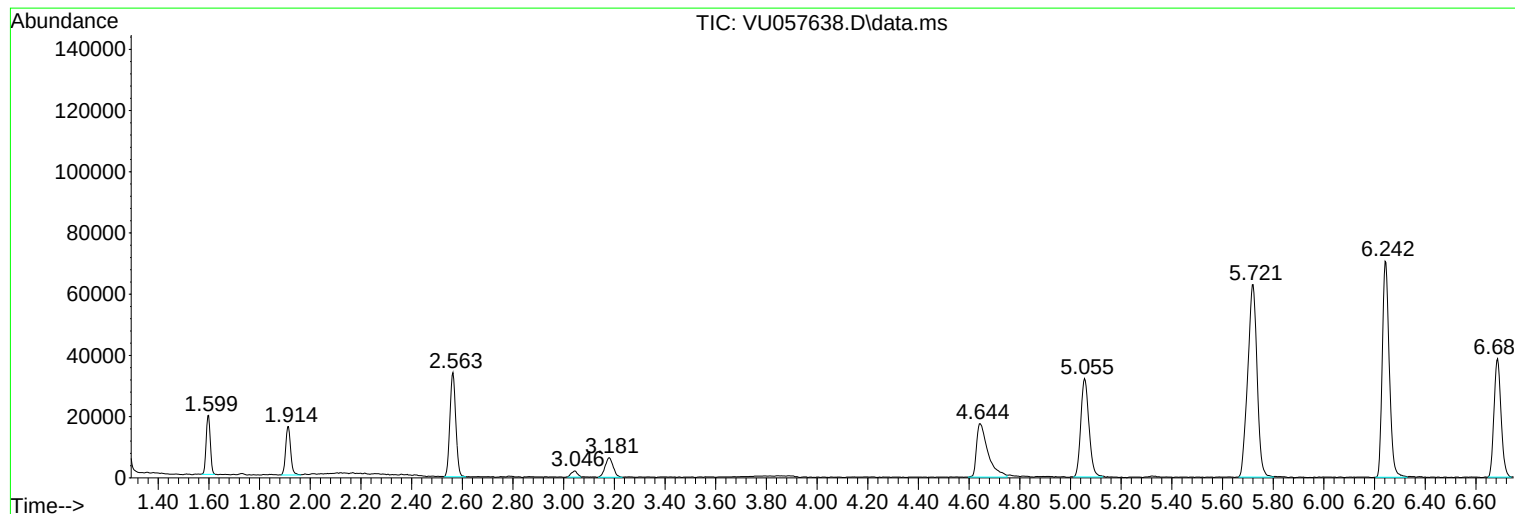

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
Data File : VU057638.D
Acq On : 24 Jan 2024 23:23
Operator : MD/SY
Sample : P1227-11DL 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B87DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
Data File : VU057638.D
Acq On : 24 Jan 2024 23:23
Operator : MD/SY
Sample : P1227-11DL 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B87DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc