

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
 Data File : VU057645.D
 Acq On : 25 Jan 2024 02:12
 Operator : MD/SY
 Sample : P1229-24 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BA9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057645.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	109	rVB	18267	21275	13.35%	1.461%
2	1.911	185	193	204	rBV	15531	20821	13.07%	1.430%
3	2.563	385	396	411	rVB	33078	53076	33.31%	3.644%
4	3.042	533	545	556	rBV2	3648	6871	4.31%	0.472%
5	3.177	574	587	606	rVB	4360	10018	6.29%	0.688%
6	4.650	1028	1045	1075	rBV	16476	56147	35.24%	3.855%
7	5.055	1158	1171	1195	rVB2	31864	72140	45.28%	4.953%
8	5.721	1360	1378	1400	rBV2	62987	159319	100.00%	10.938%
9	6.245	1528	1541	1576	rBV	66354	127484	80.02%	8.753%
10	6.685	1665	1678	1699	rBV	38472	75019	47.09%	5.151%
11	7.563	1938	1951	1965	rBV2	20038	35190	22.09%	2.416%
12	7.894	2042	2054	2080	rBV	76260	136357	85.59%	9.362%
13	8.177	2131	2142	2157	rBV2	10673	18676	11.72%	1.282%
14	8.547	2247	2257	2271	rVB	32762	55454	34.81%	3.807%
15	8.634	2273	2284	2317	rBV3	71132	155067	97.33%	10.647%
16	9.412	2515	2526	2547	rBV	85247	149390	93.77%	10.257%
17	10.749	2932	2942	2959	rBV	25155	41507	26.05%	2.850%
18	11.807	3259	3271	3292	rBV	86841	140140	87.96%	9.622%
19	12.187	3378	3389	3413	rBV	64702	107042	67.19%	7.349%
20	12.765	3559	3569	3578	rVB	3599	5464	3.43%	0.375%
21	14.572	4120	4131	4140	rVB2	6272	10047	6.31%	0.690%




Sum of corrected areas: 1456504

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
Data File : VU057645.D
Acq On : 25 Jan 2024 02:12
Operator : MD/SY
Sample : P1229-24 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

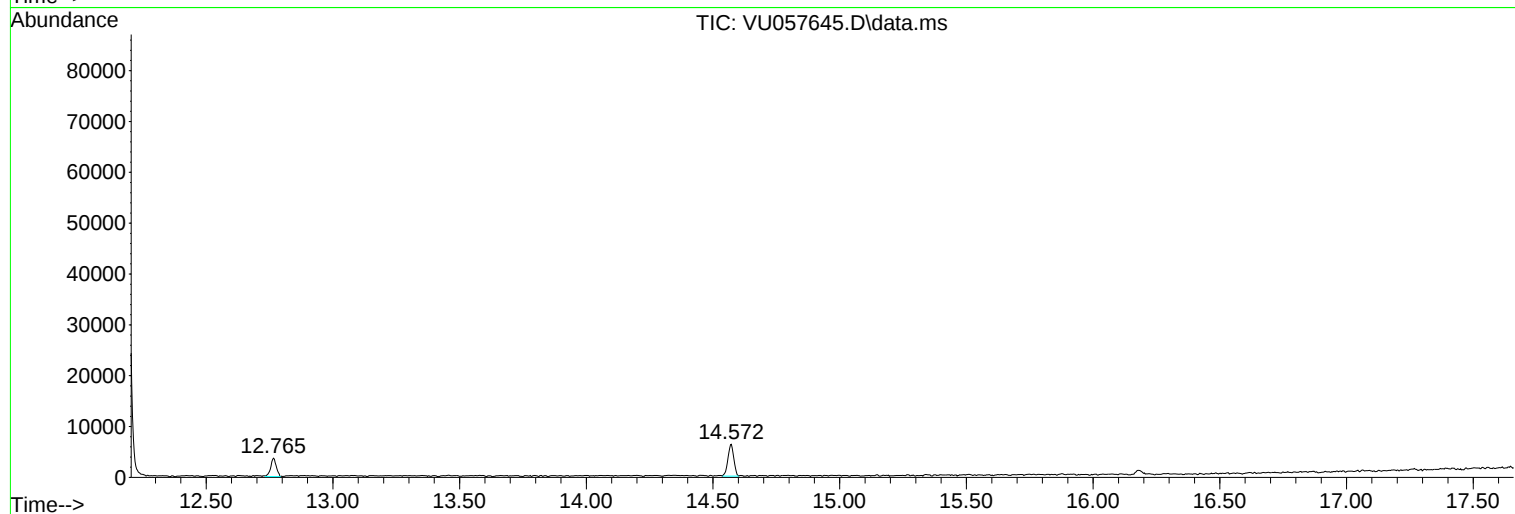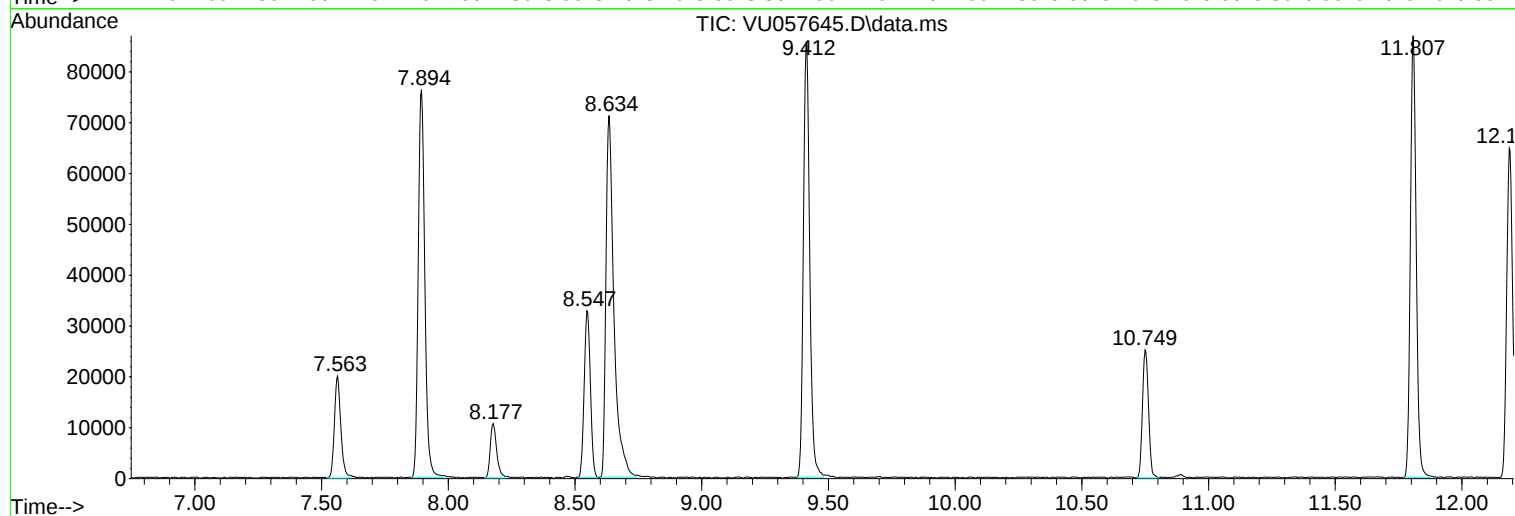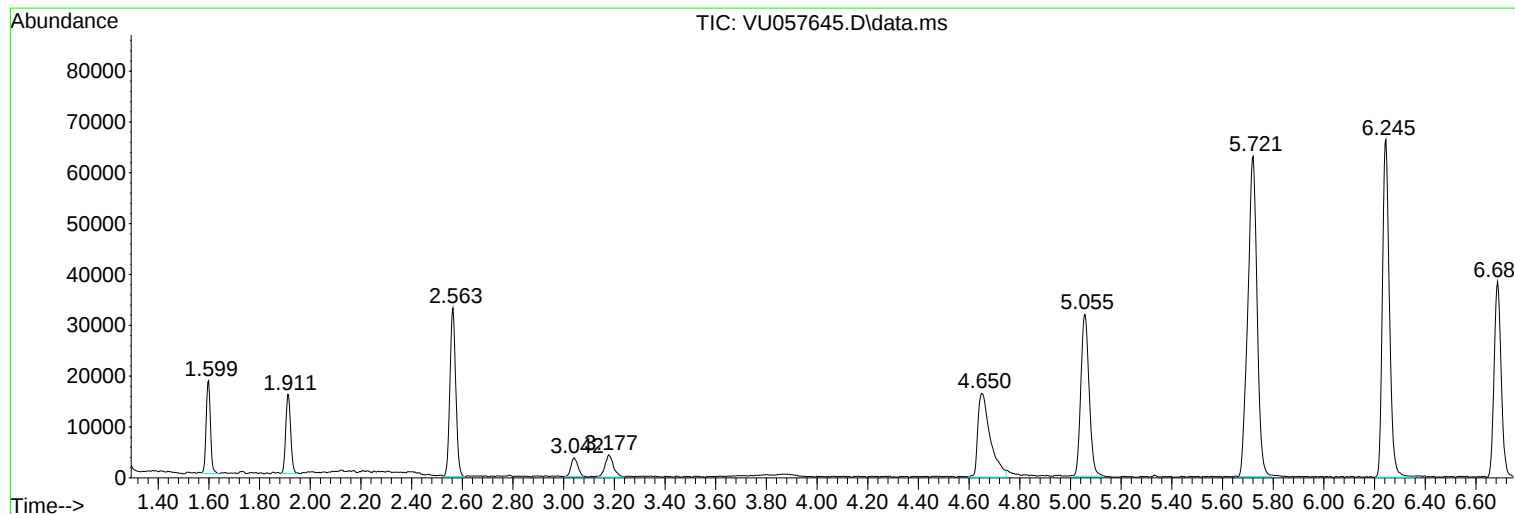

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
Data File : VU057645.D
Acq On : 25 Jan 2024 02:12
Operator : MD/SY
Sample : P1229-24 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
Data File : VU057645.D
Acq On : 25 Jan 2024 02:12
Operator : MD/SY
Sample : P1229-24 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc