

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
 Data File : VU057653.D
 Acq On : 25 Jan 2024 05:25
 Operator : MD/SY
 Sample : P1229-35 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BC0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057653.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	105	rVB	17344	19773	13.05%	1.513%
2	1.914	185	194	205	rVB	15113	19922	13.14%	1.524%
3	2.563	384	396	409	rBV	31076	50106	33.06%	3.834%
4	3.042	535	545	556	rVB2	3275	5817	3.84%	0.445%
5	3.181	574	588	602	rVB	4849	10276	6.78%	0.786%
6	4.650	1030	1045	1080	rBV	14604	51871	34.22%	3.969%
7	5.055	1157	1171	1193	rVB	30006	67313	44.41%	5.151%
8	5.721	1359	1378	1405	rBV2	59950	151569	100.00%	11.598%
9	6.245	1529	1541	1558	rBV	62029	118505	78.19%	9.068%
10	6.685	1663	1678	1696	rBV	36819	70804	46.71%	5.418%
11	7.563	1940	1951	1971	rBV2	18479	32789	21.63%	2.509%
12	7.894	2042	2054	2082	rBV	71568	126093	83.19%	9.649%
13	8.177	2133	2142	2162	rVB2	9628	16783	11.07%	1.284%
14	8.547	2253	2257	2263	rBV3	1325	1606	1.06%	0.123%
15	8.634	2273	2284	2316	rBV2	64934	144126	95.09%	11.029%
16	9.412	2515	2526	2556	rBV	81811	141170	93.14%	10.803%
17	10.749	2932	2942	2958	rBV	23130	38276	25.25%	2.929%
18	11.807	3261	3271	3291	rBV	78972	129246	85.27%	9.890%
19	12.187	3378	3389	3406	rBV	57640	96617	63.74%	7.393%
20	12.765	3559	3569	3581	rBV2	3185	4869	3.21%	0.373%
21	14.569	4121	4130	4140	rVB	5997	9288	6.13%	0.711%




Sum of corrected areas: 1306819

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
Data File : VU057653.D
Acq On : 25 Jan 2024 05:25
Operator : MD/SY
Sample : P1229-35 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

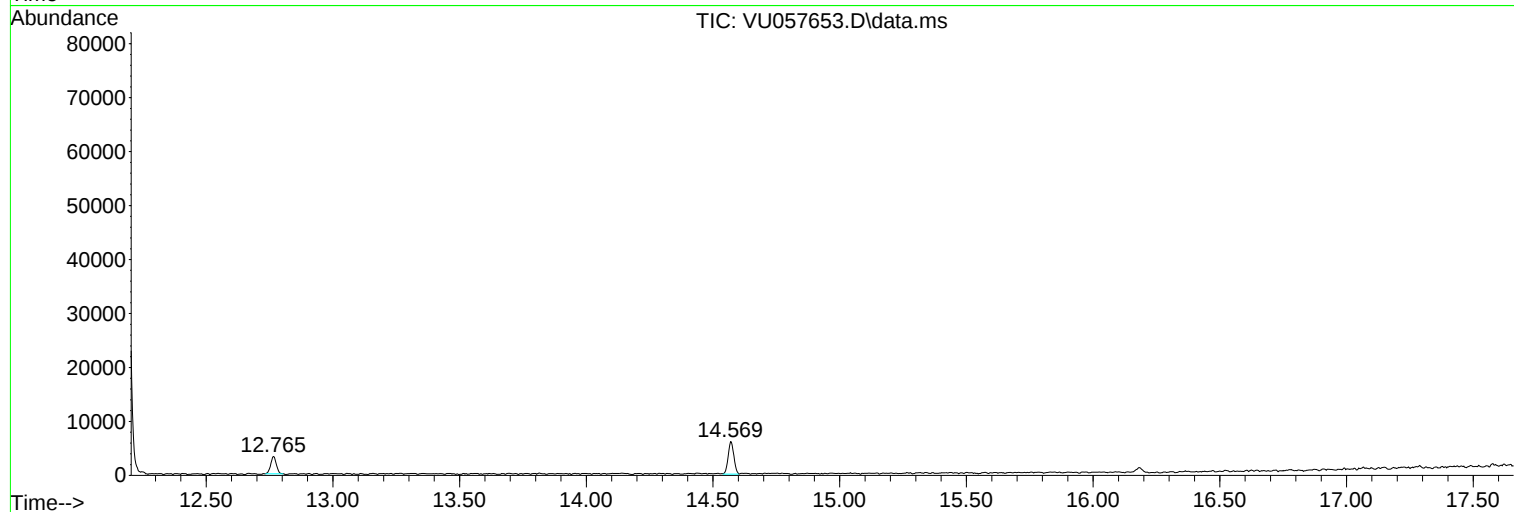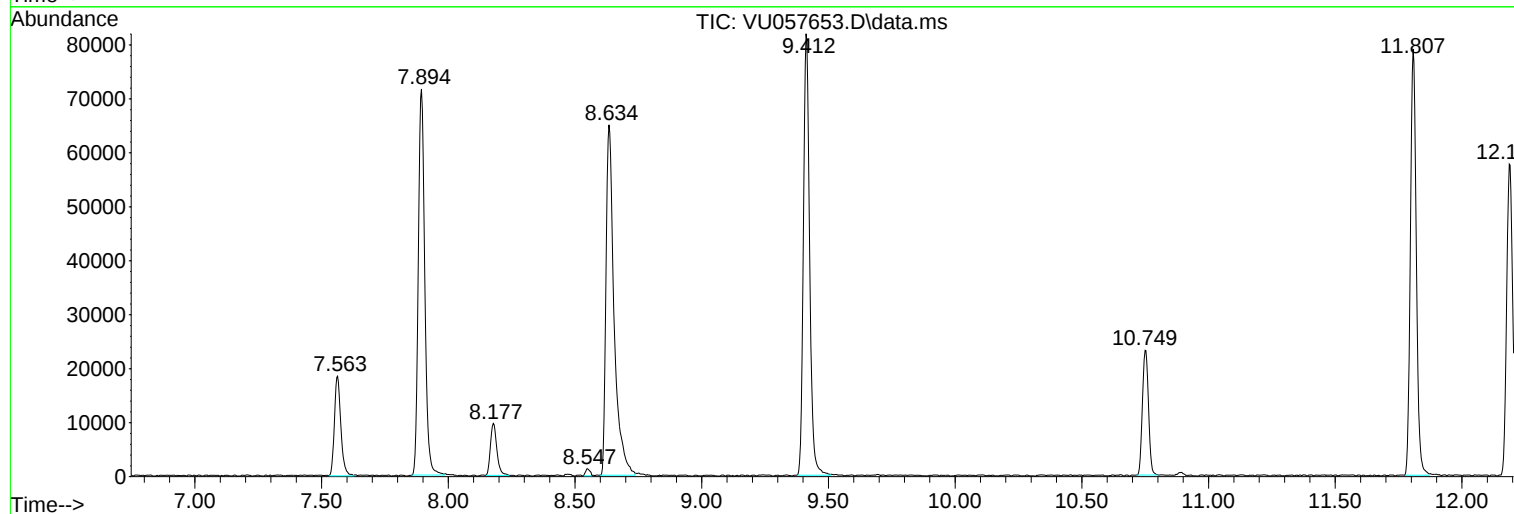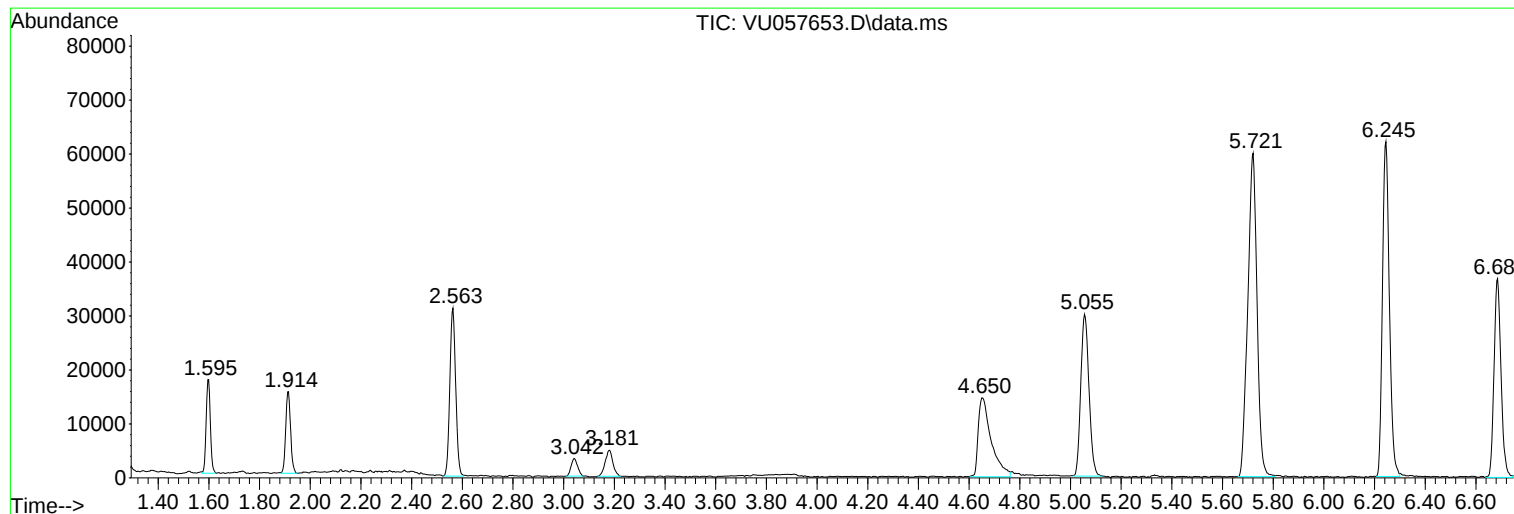

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
Data File : VU057653.D
Acq On : 25 Jan 2024 05:25
Operator : MD/SY
Sample : P1229-35 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
Data File : VU057653.D
Acq On : 25 Jan 2024 05:25
Operator : MD/SY
Sample : P1229-35 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc