


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012424\
Data File : VU057610.D
Acq On : 24 Jan 2024 09:26
Operator : MD/SY
Sample : BFB110
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB110

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Jan 30 00:30:52 2024

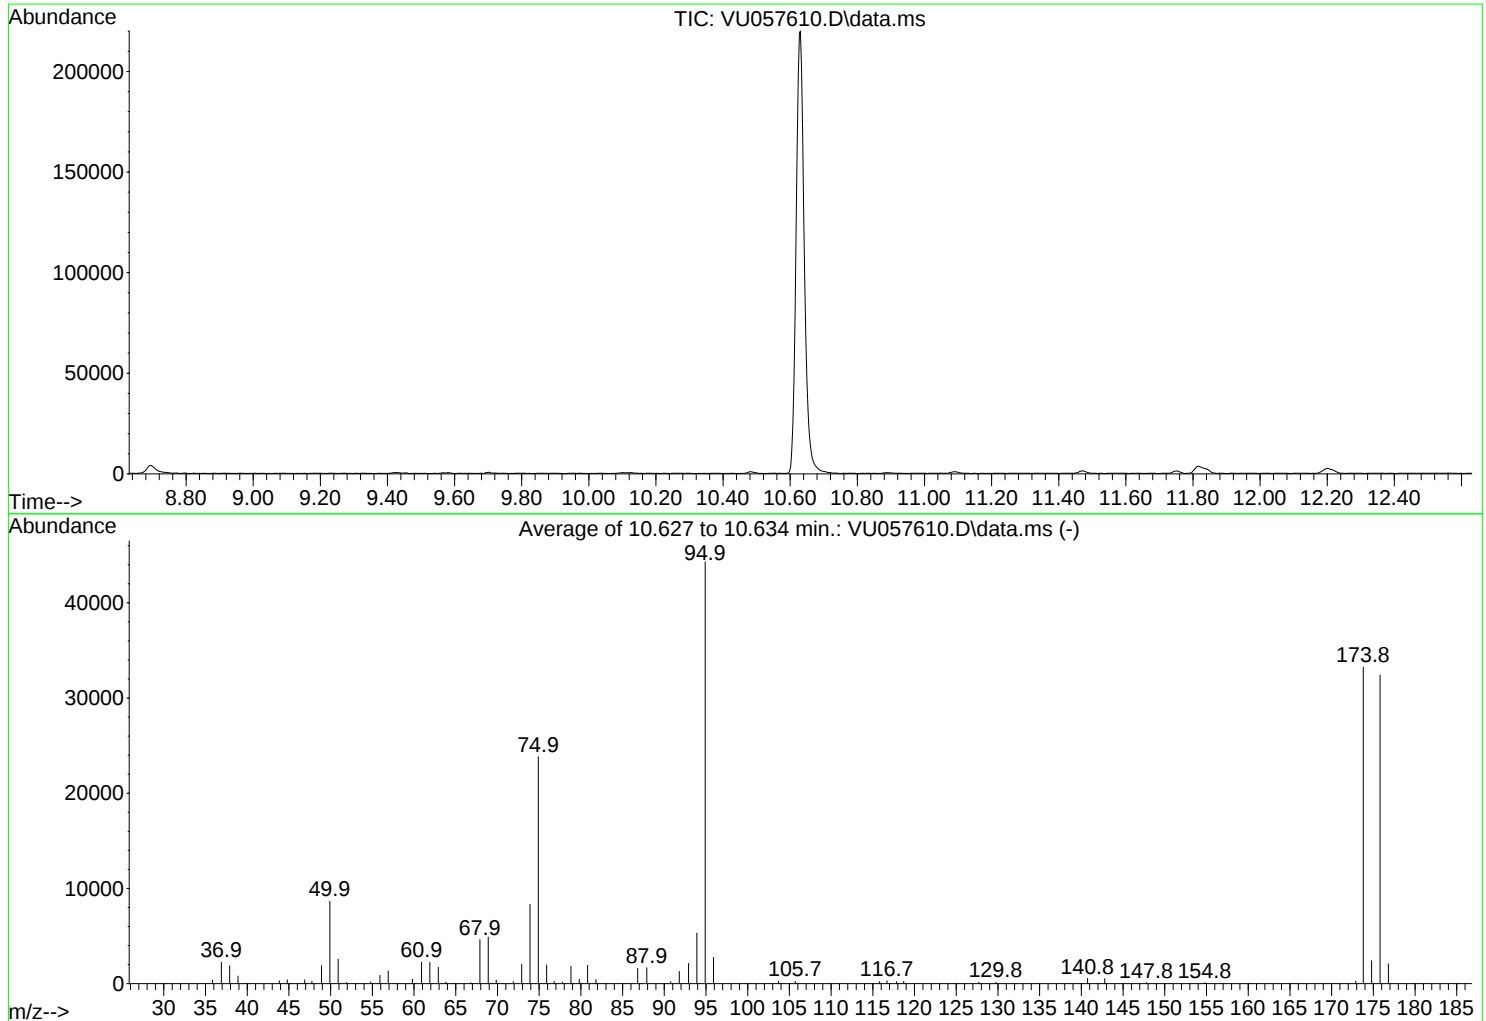

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	8640	PASS
75	95	30	80	53.8	23837	PASS
95	95	100	100	100.0	44309	PASS
96	95	5	9	6.2	2762	PASS
173	174	0.00	2	0.8	275	PASS
174	95	50	120	75.0	33240	PASS
175	174	5	9	7.2	2396	PASS
176	174	95	101	97.5	32419	PASS
177	176	5	9	6.4	2078	PASS

m/z	Abundance
39.80	115.0
43.80	171.0

Instrument :
MSVOA_U
ClientSampleId :
BFB110

m/z	Abundance
35.90	392.0
36.90	2321.0
37.90	2008.0
38.90	814.0
39.80	116.0
43.90	463.0
44.80	421.0
46.90	421.0
47.80	267.0
48.90	2014.0
49.90	8928.0
50.90	2674.0
51.90	117.0
54.80	177.0
55.90	881.0
56.90	1449.0
59.80	490.0
60.90	2374.0
61.90	2298.0
62.90	1770.0
63.80	173.0
66.80	164.0
67.90	4803.0
68.90	5035.0
69.90	356.0
71.90	232.0
72.90	2059.0
73.90	8687.0
74.90	24784.0
75.90	2041.0
76.80	222.0
77.80	194.0
78.80	1906.0
79.80	495.0
80.80	2012.0
81.80	404.0
86.80	1664.0
87.90	1649.0
90.70	182.0
91.80	1343.0
92.90	2134.0
93.90	5427.0
94.90	45608.0
95.90	2863.0
103.70	245.0
105.70	274.0
115.80	190.0
116.70	315.0
117.80	195.0
118.70	295.0
127.70	153.0
129.80	170.0
140.80	563.0
142.80	539.0
147.80	125.0
154.80	118.0
172.90	286.0
173.80	33560.0
174.80	2428.0
175.80	32560.0
176.80	2106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB110

m/z	Abundance
35.80	389.0
36.90	2331.0
37.90	1903.0
38.90	829.0
39.70	111.0
43.90	483.0
44.80	423.0
46.90	428.0
47.70	266.0
48.90	1962.0
49.90	8897.0
50.90	2656.0
51.90	115.0
54.80	195.0
55.90	899.0
56.90	1383.0
59.80	499.0
60.90	2276.0
61.90	2329.0
62.90	1781.0
63.80	168.0
66.80	130.0
67.90	4750.0
68.90	5019.0
69.80	396.0
71.90	237.0
72.90	2070.0
73.90	8585.0
74.90	24584.0
75.90	2022.0
76.80	236.0
77.80	176.0
78.80	1878.0
79.80	496.0
80.80	1971.0
81.80	425.0
86.80	1640.0
87.90	1711.0
90.80	201.0
91.80	1328.0
92.90	2205.0
93.90	5439.0
94.90	45728.0
95.90	2844.0
103.70	260.0
105.70	263.0
115.80	209.0
116.70	312.0
117.90	212.0
118.70	263.0
127.70	164.0
129.80	163.0
140.80	566.0
142.80	534.0
147.80	125.0
154.80	120.0
172.90	283.0
173.80	34168.0
174.80	2462.0
175.80	33408.0
176.80	2141.0

Instrument :
MSVOA_U
ClientSampleId :
BFB110

m/z	Abundance
35.80	350.0
36.90	2077.0
37.90	1675.0
38.90	748.0
39.80	114.0
43.90	488.0
44.80	386.0
46.90	390.0
47.80	233.0
48.90	1739.0
49.90	8095.0
50.90	2386.0
51.90	103.0
54.80	172.0
55.90	824.0
56.90	1201.0
59.80	443.0
60.90	2094.0
61.90	2105.0
62.90	1615.0
63.80	161.0
67.90	4329.0
68.90	4615.0
69.90	382.0
71.90	208.0
72.90	1921.0
73.90	7671.0
74.90	22144.0
75.90	1859.0
76.80	225.0
77.80	162.0
78.80	1719.0
79.80	447.0
80.80	1771.0
81.80	420.0
86.80	1517.0
87.90	1632.0
90.80	211.0
91.80	1173.0
92.90	2029.0
93.90	5081.0
94.90	41592.0
95.90	2578.0
103.70	260.0
105.70	236.0
115.80	191.0
116.70	296.0
117.90	197.0
118.70	213.0
127.70	158.0
129.70	150.0
140.70	522.0
142.80	487.0
147.80	110.0
154.80	105.0
172.90	257.0
173.80	31992.0
174.80	2298.0
175.80	31288.0
176.80	1987.0

Instrument :
MSVOA_U
ClientSampleId :
BFB110