

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012524\
 Data File : VU057661.D
 Acq On : 25 Jan 2024 12:22
 Operator : MD/SY
 Sample : P1227-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B90

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057661.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	106	rVB	19326	22183	11.95%	1.467%
2	1.911	185	193	207	rBV	16202	21490	11.58%	1.421%
3	2.563	385	396	411	rVB	34209	54409	29.31%	3.597%
4	3.181	576	588	598	rBV	3924	8722	4.70%	0.577%
5	3.268	602	615	641	rVB5	2587	12144	6.54%	0.803%
6	4.634	1027	1040	1076	rBV	19528	57475	30.96%	3.800%
7	5.055	1158	1171	1195	rBV	32955	72406	39.01%	4.787%
8	5.721	1360	1378	1409	rBV2	64402	162852	87.73%	10.768%
9	6.245	1529	1541	1567	rBV	81025	155433	83.74%	10.277%
10	6.685	1663	1678	1696	rBV	39871	75733	40.80%	5.007%
11	7.563	1940	1951	1969	rBV2	20047	35330	19.03%	2.336%
12	7.894	2042	2054	2074	rBV	81488	142643	76.85%	9.431%
13	8.177	2132	2142	2161	rBV2	10849	18805	10.13%	1.243%
14	8.550	2252	2258	2266	rVB3	1792	2414	1.30%	0.160%
15	8.634	2270	2284	2318	rBV3	69516	150336	80.99%	9.940%
16	9.412	2514	2526	2548	rBV	107197	185619	100.00%	12.273%
17	10.753	2932	2943	2960	rBV	25383	40642	21.90%	2.687%
18	11.807	3260	3271	3292	rBV	107336	172867	93.13%	11.430%
19	12.187	3378	3389	3410	rBV	67566	112611	60.67%	7.446%
20	12.766	3559	3569	3585	rVB	5421	8300	4.47%	0.549%




Sum of corrected areas: 1512414

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012524\
Data File : VU057661.D
Acq On : 25 Jan 2024 12:22
Operator : MD/SY
Sample : P1227-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

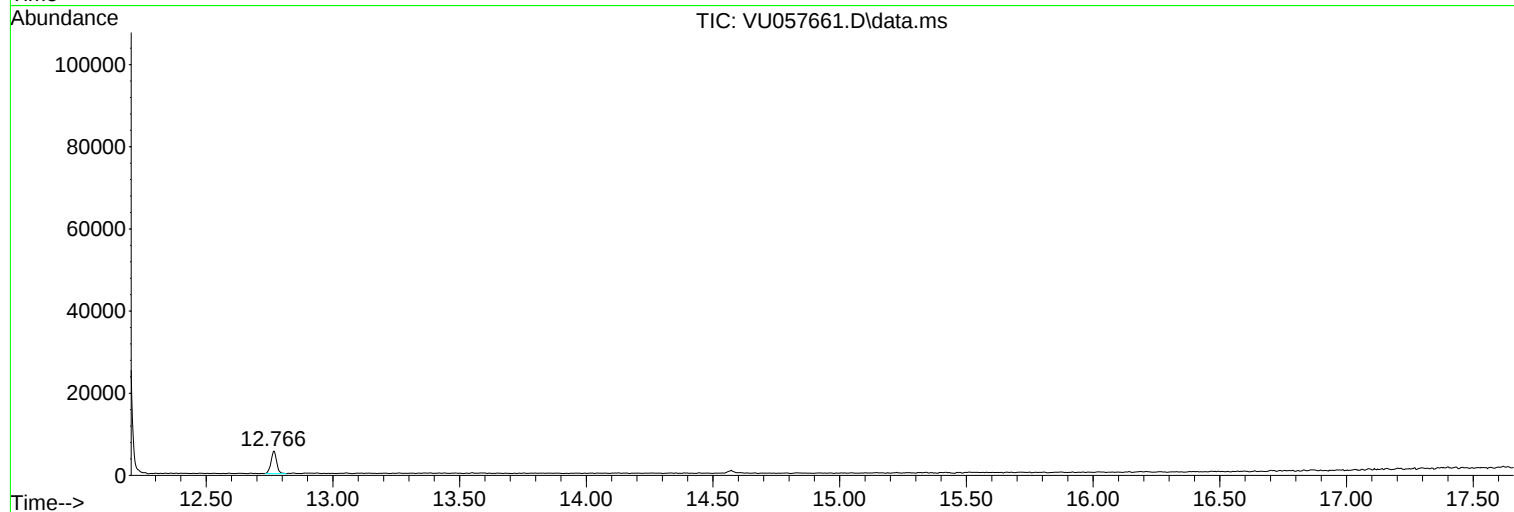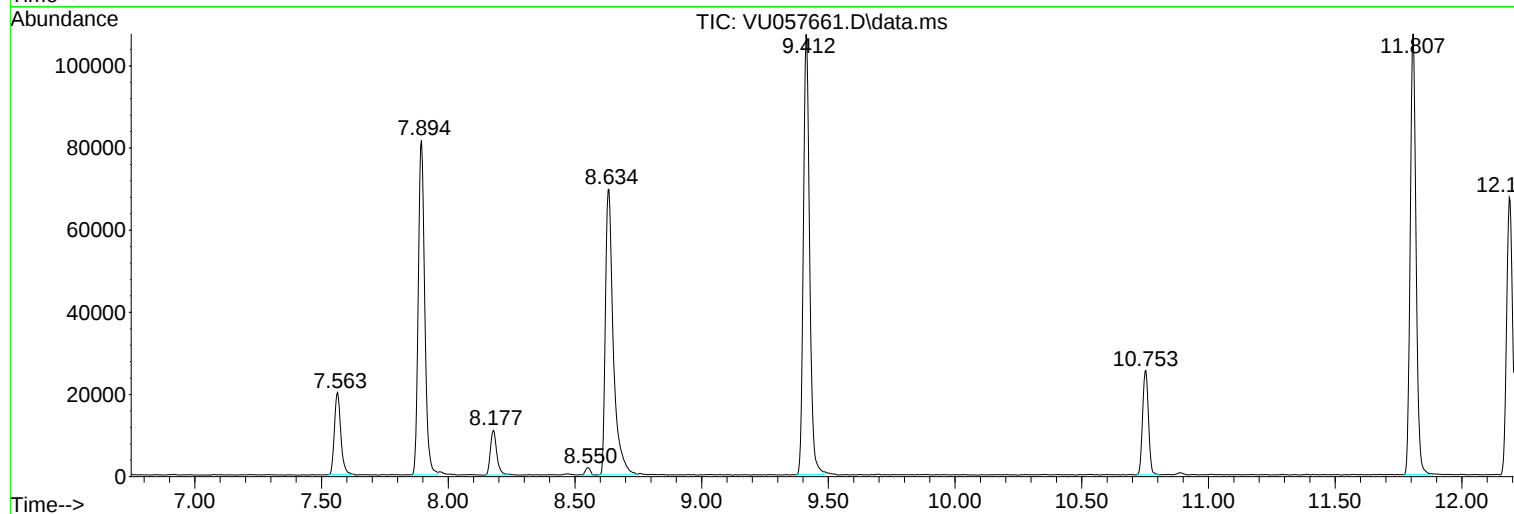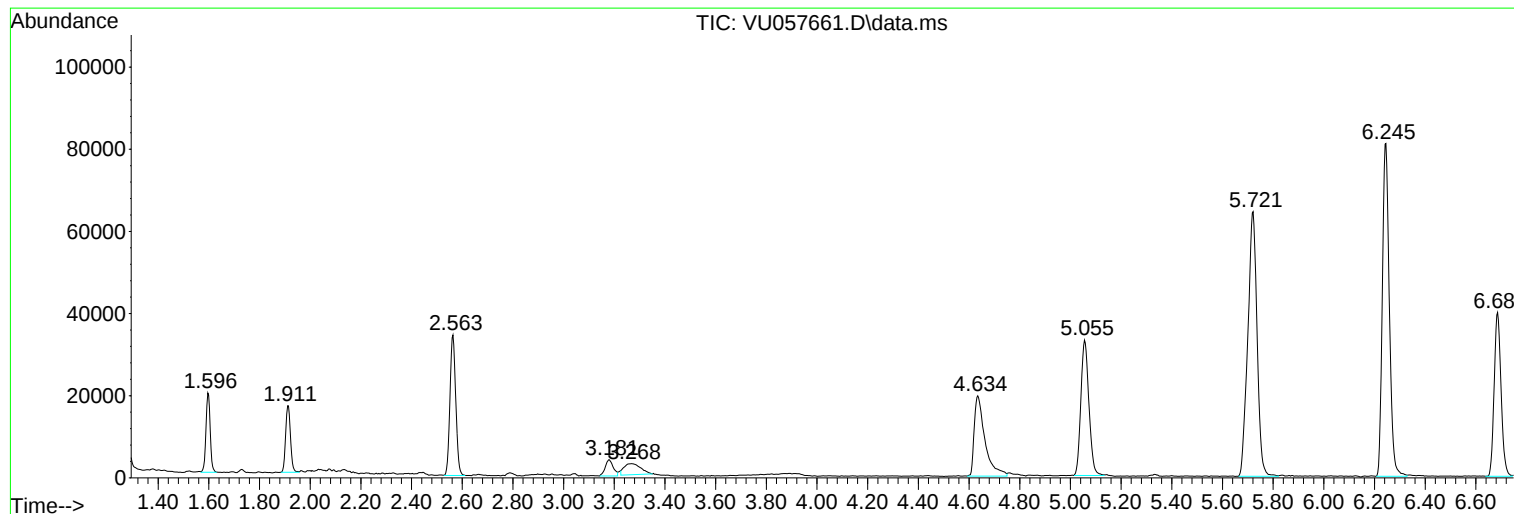

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012524\
Data File : VU057661.D
Acq On : 25 Jan 2024 12:22
Operator : MD/SY
Sample : P1227-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012524\
Data File : VU057661.D
Acq On : 25 Jan 2024 12:22
Operator : MD/SY
Sample : P1227-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc