


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012524\
Data File : VU057655.D
Acq On : 25 Jan 2024 09:13
Operator : MD/SY
Sample : BFB111
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB111

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Jan 30 00:30:52 2024

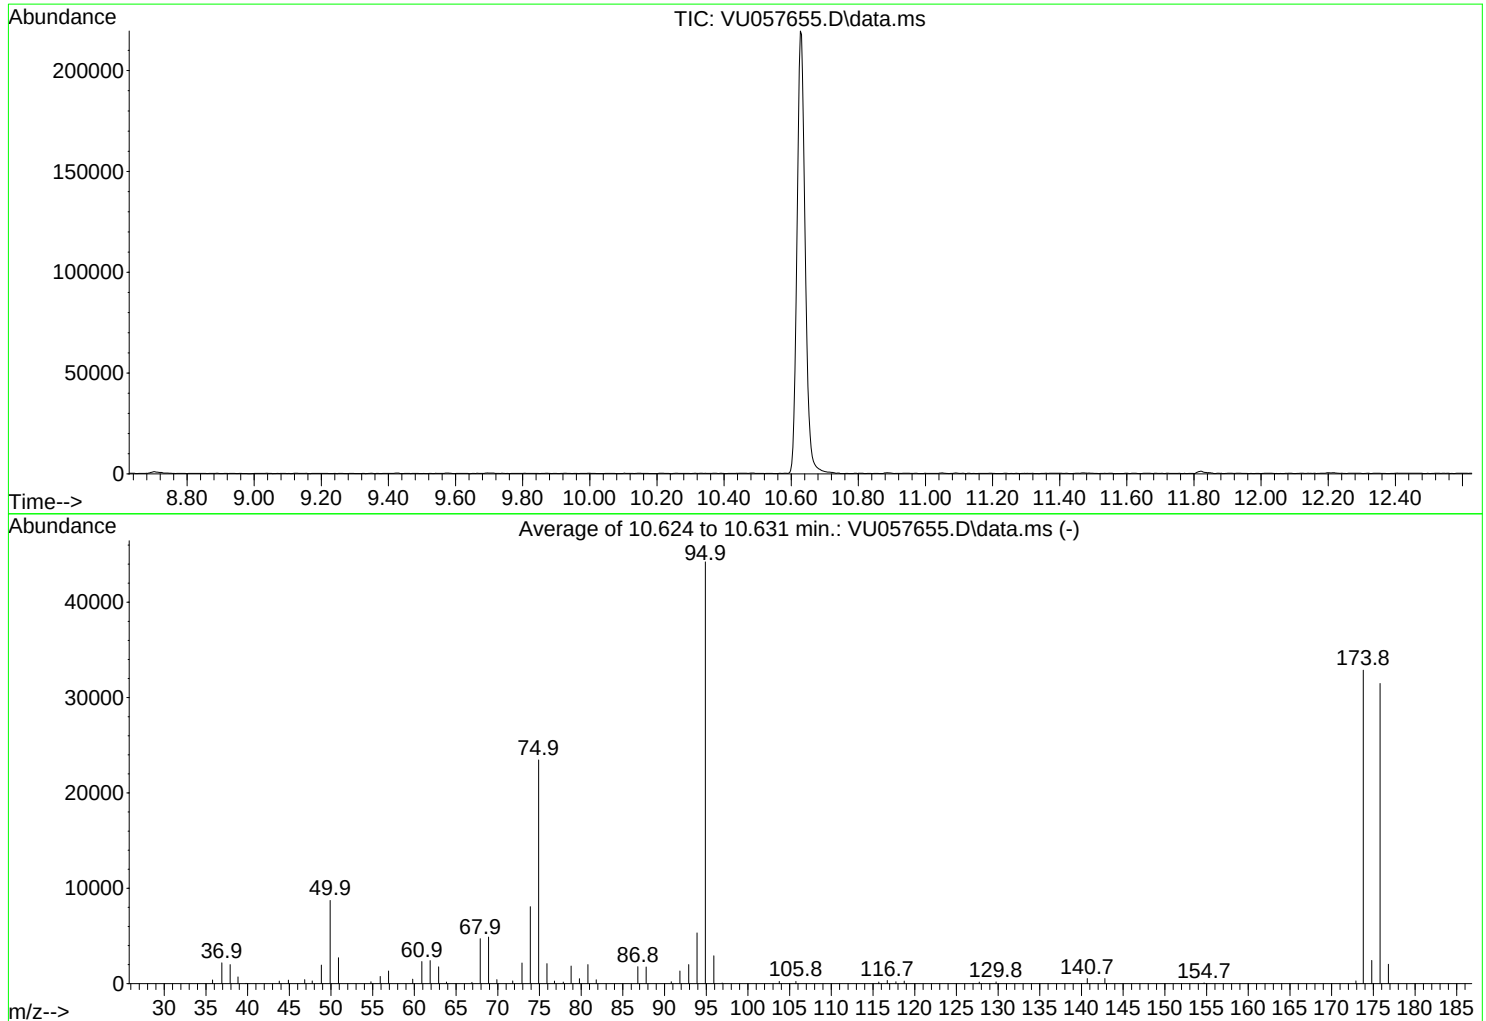

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	8730	PASS
75	95	30	80	53.0	23459	PASS
95	95	100	100	100.0	44240	PASS
96	95	5	9	6.6	2925	PASS
173	174	0.00	2	0.9	285	PASS
174	95	50	120	74.3	32885	PASS
175	174	5	9	7.4	2427	PASS
176	174	95	101	95.7	31485	PASS
177	176	5	9	6.5	2035	PASS

Scan 2891 (10.586 min): VU057655.D\data.ms
BFB111

m/z	Abundance
39.90	130.0
43.80	168.0

Instrument :
MSVOA_U
ClientSampleId :
BFB111

m/z	Abundance
35.80	367.0
36.90	2046.0
37.90	1933.0
38.90	657.0
39.80	156.0
43.90	416.0
44.90	355.0
46.90	370.0
47.80	254.0
48.90	1870.0
49.90	8517.0
50.90	2652.0
54.80	195.0
55.90	734.0
56.90	1194.0
59.80	462.0
60.90	2166.0
61.90	2306.0
62.90	1671.0
63.80	182.0
66.90	110.0
67.90	4567.0
68.90	4610.0
69.90	413.0
71.80	267.0
72.90	2073.0
73.90	7678.0
74.90	22432.0
75.90	2059.0
76.80	250.0
77.80	159.0
78.80	1778.0
79.80	489.0
80.80	1931.0
81.80	394.0
86.80	1693.0
87.80	1630.0
90.80	169.0
91.90	1293.0
92.90	1867.0
93.90	5034.0
94.90	42112.0
95.90	2849.0
96.90	100.0
103.80	236.0
105.70	229.0
115.70	161.0
116.70	327.0
117.70	199.0
118.70	261.0
127.70	177.0
129.70	176.0
140.70	448.0
142.80	456.0
172.90	272.0
173.80	30384.0
174.80	2306.0
175.80	29152.0
176.80	1894.0

Instrument :
MSVOA_U
ClientSampleId :
BFB111

m/z	Abundance
35.80	399.0
36.90	2249.0
37.90	2055.0
38.90	730.0
39.80	173.0
43.80	433.0
44.90	375.0
46.80	407.0
47.80	279.0
48.90	2008.0
49.90	8975.0
50.90	2796.0
54.80	205.0
55.90	760.0
56.90	1362.0
59.80	485.0
60.90	2396.0
61.90	2500.0
62.90	1808.0
63.90	181.0
66.90	145.0
67.90	4905.0
68.90	5019.0
69.90	429.0
71.80	288.0
72.90	2231.0
73.90	8329.0
74.90	24160.0
75.90	2187.0
76.80	284.0
77.80	161.0
78.80	1915.0
79.80	535.0
80.80	2072.0
81.80	422.0
86.80	1867.0
87.80	1829.0
90.80	202.0
91.90	1382.0
92.90	2056.0
93.90	5467.0
94.90	45600.0
95.90	3011.0
96.90	106.0
103.70	242.0
105.80	242.0
115.70	168.0
116.70	342.0
117.80	198.0
118.70	272.0
127.70	175.0
129.80	196.0
140.70	554.0
142.80	547.0
154.70	118.0
172.90	288.0
173.80	33928.0
174.80	2503.0
175.80	32552.0
176.80	2094.0

Instrument :
MSVOA_U
ClientSampleId :
BFB111

m/z	Abundance
35.80	383.0
36.90	2231.0
37.90	2014.0
38.80	743.0
39.80	181.0
43.80	449.0
44.90	379.0
46.80	463.0
47.70	302.0
48.80	1972.0
49.90	8699.0
50.90	2715.0
54.80	191.0
55.90	750.0
56.90	1441.0
59.80	455.0
60.90	2408.0
61.90	2445.0
62.90	1788.0
63.90	165.0
66.90	166.0
67.90	4703.0
68.90	5016.0
69.90	410.0
71.80	291.0
72.90	2204.0
73.90	8198.0
74.90	23784.0
75.90	2075.0
76.80	274.0
77.90	161.0
78.80	1854.0
79.80	522.0
80.80	2001.0
81.80	407.0
86.80	1781.0
87.80	1788.0
90.80	218.0
91.80	1314.0
92.90	2068.0
93.90	5469.0
94.90	45008.0
95.90	2914.0
103.70	237.0
105.80	246.0
115.70	159.0
116.70	321.0
117.80	206.0
118.80	257.0
127.80	167.0
129.80	192.0
140.70	600.0
142.80	587.0
154.70	123.0
172.90	296.0
173.80	34344.0
174.80	2472.0
175.80	32752.0
176.80	2118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB111