
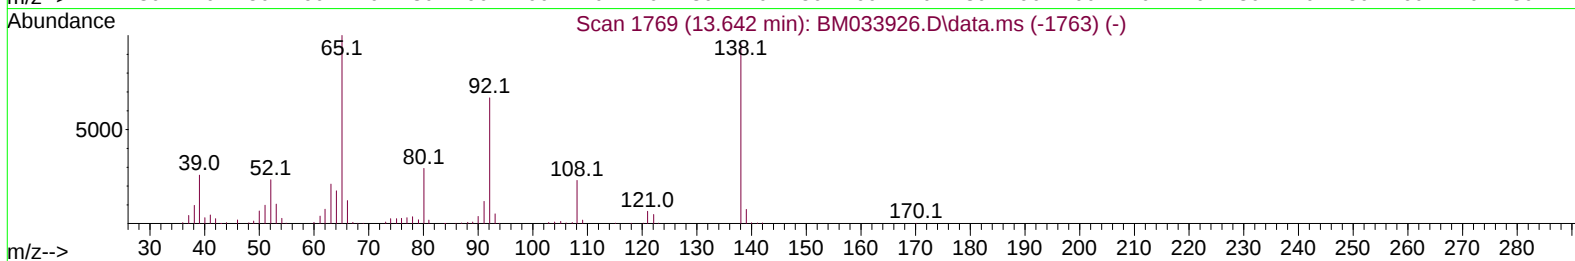
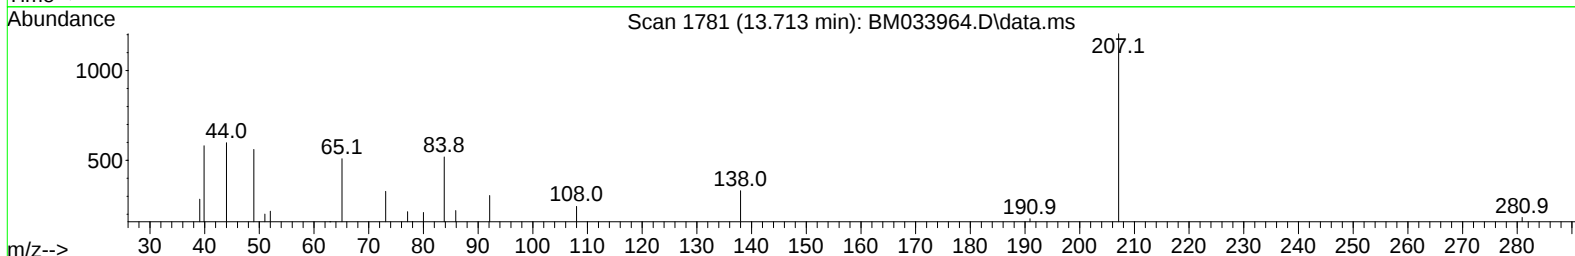


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033964.D
 Acq On : 02 Feb 2022 06:58
 Operator : CG/JU
 Sample : SSTCCCC020
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Quant Time: Feb 02 12:58:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

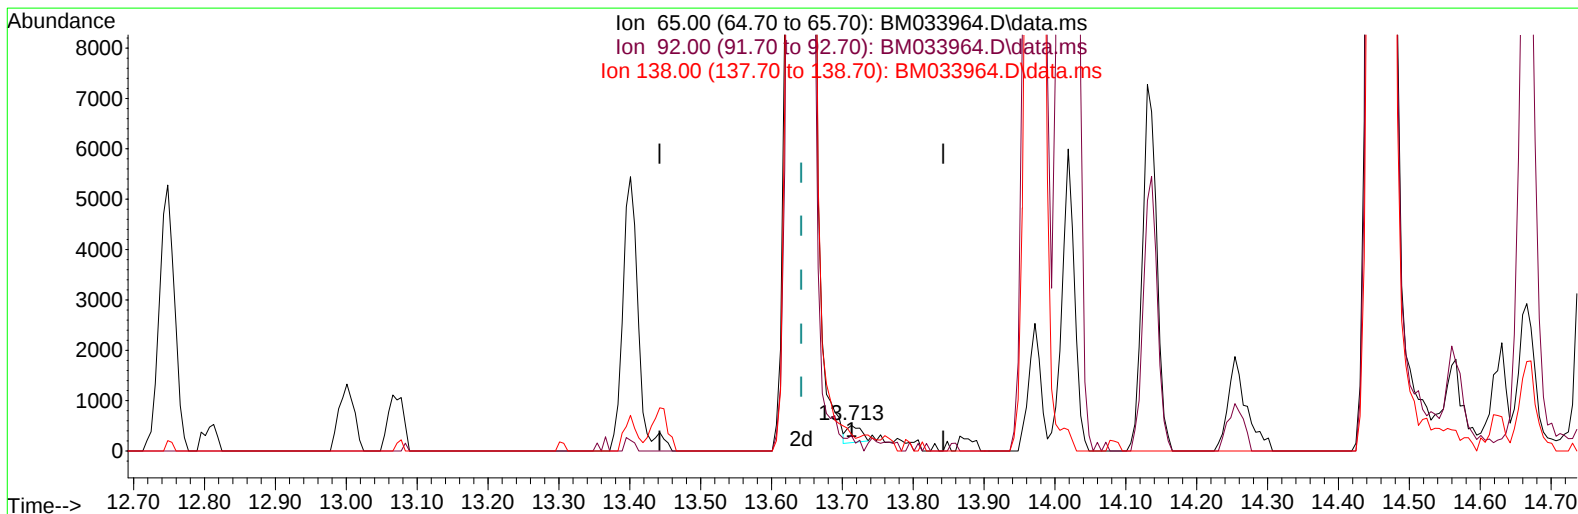

TIC: BM033964.D\data.ms

(45) 2-Nitroaniline

13.713min (+ 0.071) 0.06 ng/u1

response 475

Ion	Exp%	Act%
65.00	100.00	100.00
92.00	59.70	59.72
138.00	76.30	65.03
0.00	0.00	0.00