

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020122\
 Data File : VU046964.D
 Acq On : 01 Feb 2022 15:11
 Operator : SY/MD
 Sample : N1328-15 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HN4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU046964.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	111	rVB	50753	80261	4.33%	1.299%
2	1.919	172	180	191	rBV	34889	52356	2.82%	0.848%
3	2.565	368	381	400	rBV3	128295	241018	12.99%	3.902%
4	4.668	1016	1035	1071	rBV2	157492	456273	24.59%	7.386%
5	5.067	1143	1159	1182	rBV	78195	174484	9.40%	2.825%
6	5.314	1223	1236	1257	rVB2	17672	40045	2.16%	0.648%
7	5.726	1344	1364	1389	rBV2	162125	415393	22.39%	6.725%
8	6.250	1511	1527	1554	rBV	127752	249010	13.42%	4.031%
9	6.543	1603	1618	1634	rBV	207073	385850	20.79%	6.246%
10	6.694	1652	1665	1685	rVB	97523	191622	10.33%	3.102%
11	7.568	1925	1937	1953	rBV	45348	79748	4.30%	1.291%
12	7.899	2027	2040	2061	rBV	163094	306557	16.52%	4.963%
13	8.182	2114	2128	2141	rBV2	27147	49161	2.65%	0.796%
14	8.555	2229	2244	2262	rBV	1064254	1855607	100.00%	30.040%
15	8.658	2262	2276	2307	rVB	219969	532808	28.71%	8.625%
16	9.420	2500	2513	2536	rBV	194322	357098	19.24%	5.781%
17	10.764	2918	2931	2946	rVB	85247	142438	7.68%	2.306%
18	11.816	3245	3258	3276	rBV	198065	310016	16.71%	5.019%
19	12.195	3361	3376	3393	rBV	160852	257468	13.88%	4.168%




Sum of corrected areas: 6177213

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020122\
Data File : VU046964.D
Acq On : 01 Feb 2022 15:11
Operator : SY/MD
Sample : N1328-15 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COHN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

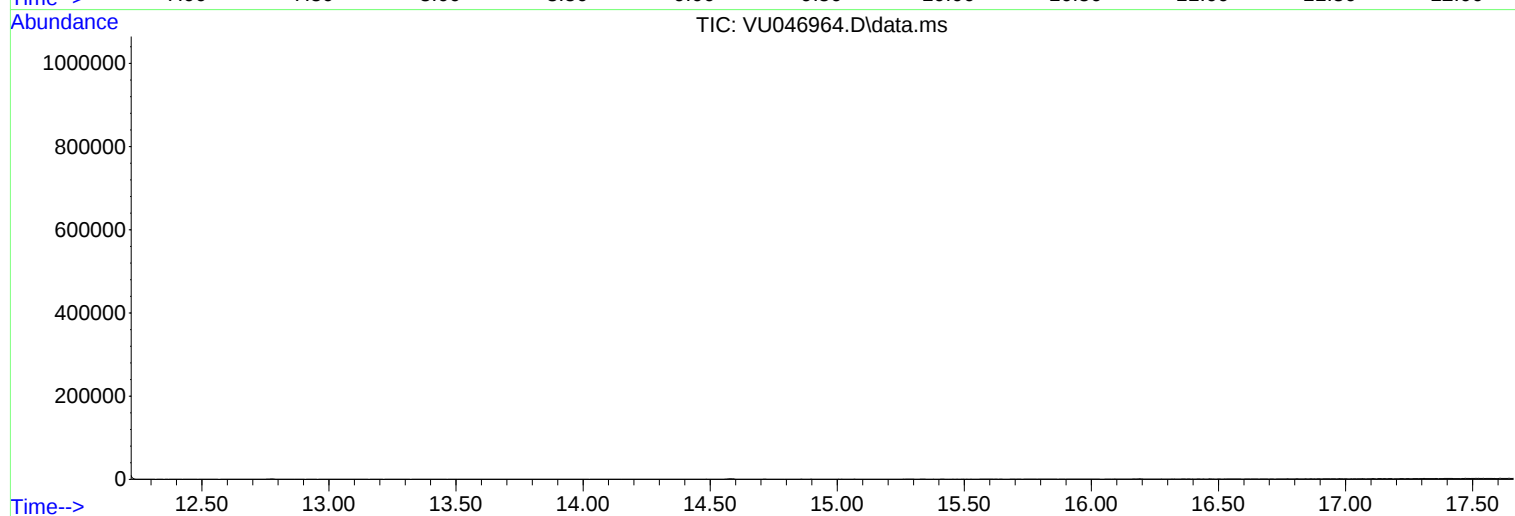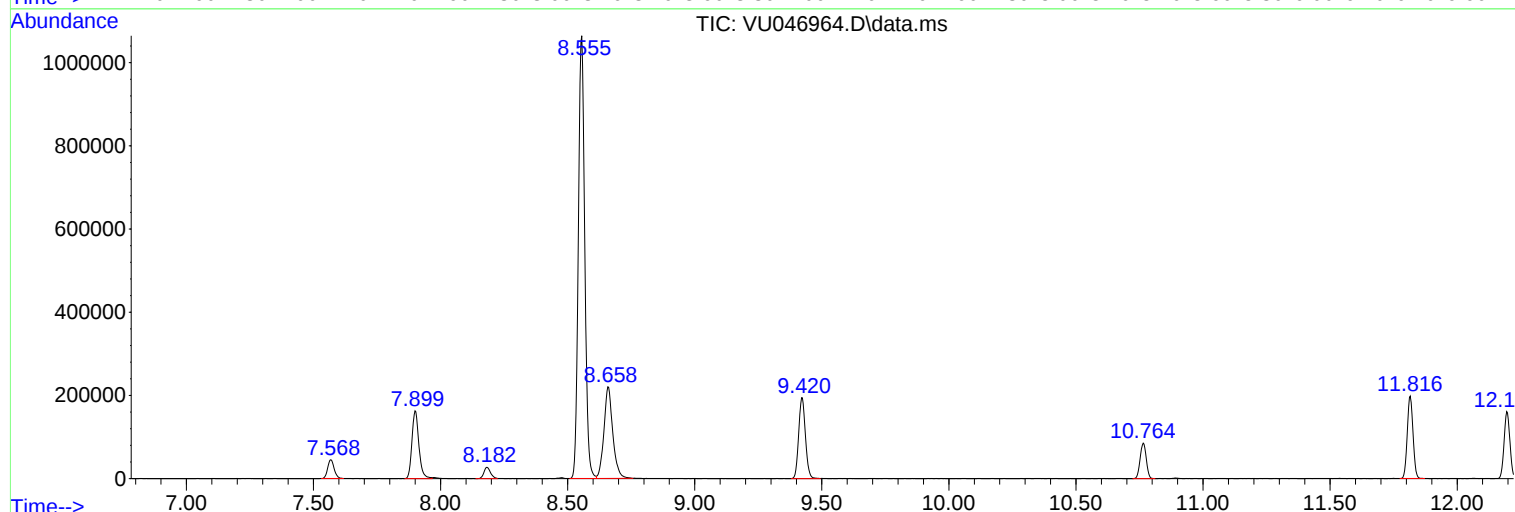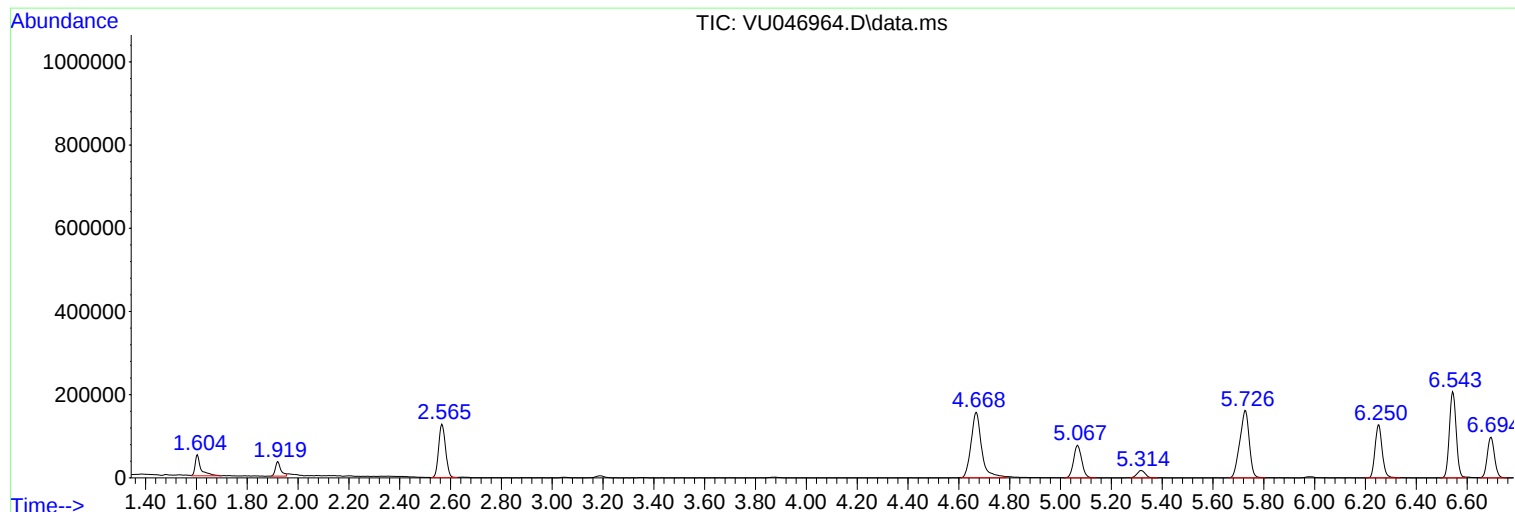

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020122\
Data File : VU046964.D
Acq On : 01 Feb 2022 15:11
Operator : SY/MD
Sample : N1328-15 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020122\
Data File : VU046964.D
Acq On : 01 Feb 2022 15:11
Operator : SY/MD
Sample : N1328-15 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc