

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020122\
 Data File : VU046974.D
 Acq On : 01 Feb 2022 19:28
 Operator : SY/MD
 Sample : N1273-21 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHL9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU046974.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	73	82	96	rBV2	86535	106097	10.74%	1.731%
2	1.919	172	180	196	rVB	48777	65131	6.60%	1.062%
3	2.584	368	387	411	rBV3	461210	834742	84.53%	13.616%
4	3.877	775	789	806	rVB	10077	23207	2.35%	0.379%
5	4.671	1014	1036	1063	rBV2	177914	505438	51.18%	8.245%
6	5.067	1145	1159	1178	rVB	79069	172925	17.51%	2.821%
7	5.321	1226	1238	1250	rVB3	5367	11035	1.12%	0.180%
8	5.729	1344	1365	1383	rBV2	154617	407610	41.27%	6.649%
9	6.253	1513	1528	1544	rBV	118988	228203	23.11%	3.722%
10	6.546	1604	1619	1646	rBV	530988	987559	100.00%	16.109%
11	6.694	1652	1665	1682	rVB	100210	194366	19.68%	3.171%
12	7.568	1924	1937	1956	rBV	45765	80185	8.12%	1.308%
13	7.899	2028	2040	2060	rBV	162634	299885	30.37%	4.892%
14	8.182	2115	2128	2145	rBV2	28249	48621	4.92%	0.793%
15	8.555	2231	2244	2259	rBV	390374	681462	69.00%	11.116%
16	8.636	2259	2269	2314	rVB	225654	484047	49.01%	7.896%
17	9.420	2499	2513	2538	rBV	193433	333996	33.82%	5.448%
18	10.758	2917	2929	2945	rVB2	82398	132406	13.41%	2.160%
19	11.812	3245	3257	3276	rVB	178774	284883	28.85%	4.647%
20	12.195	3364	3376	3392	rBV	154443	248579	25.17%	4.055%




Sum of corrected areas: 6130377

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020122\
Data File : VU046974.D
Acq On : 01 Feb 2022 19:28
Operator : SY/MD
Sample : N1273-21 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

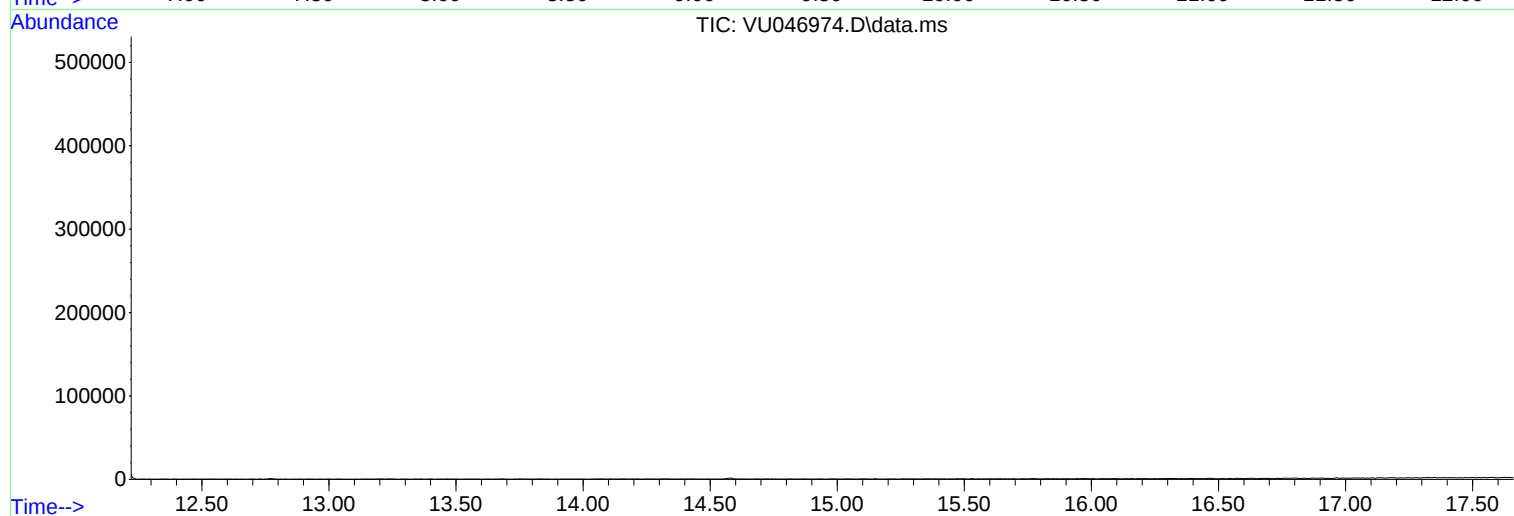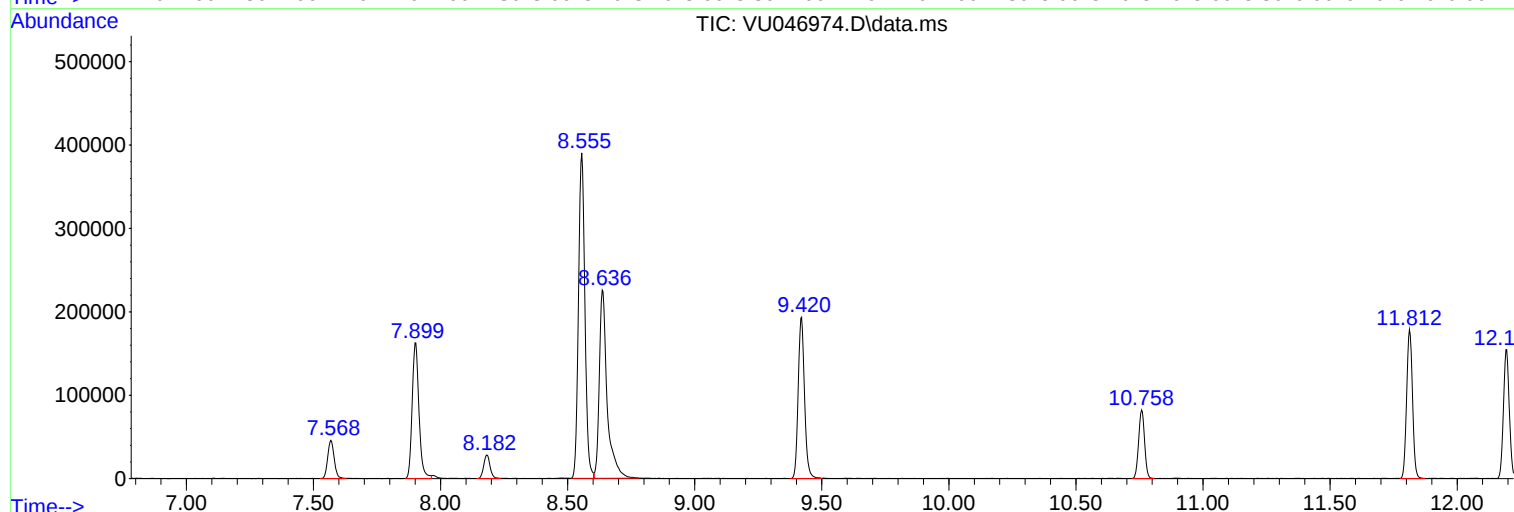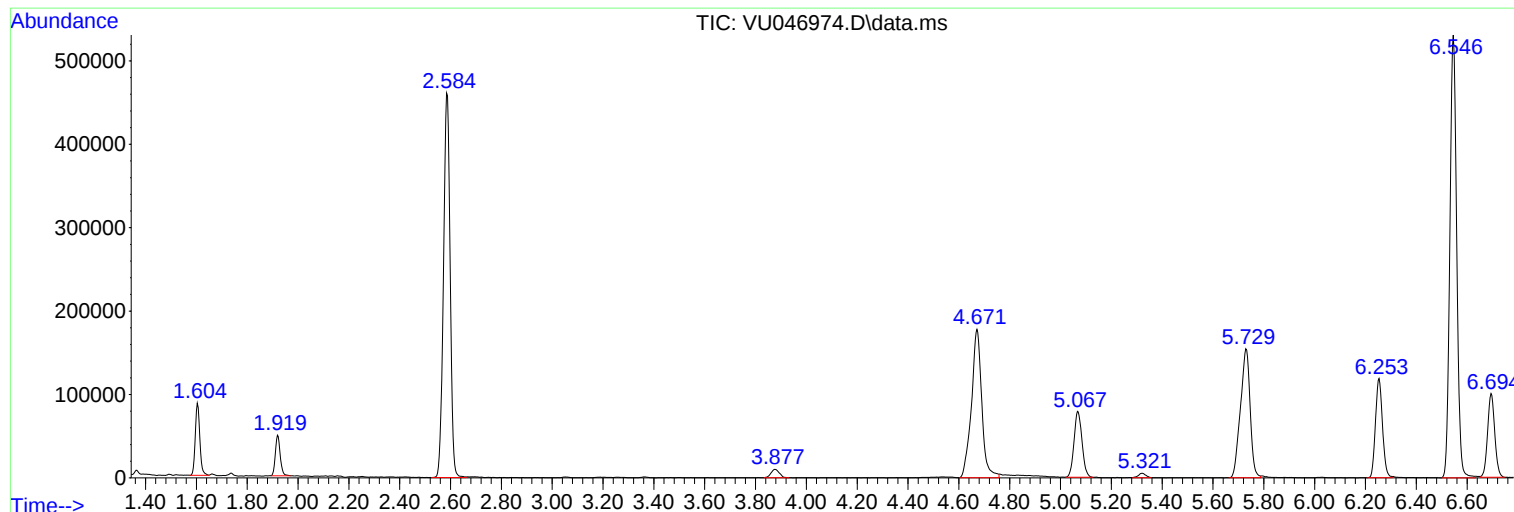

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020122\
Data File : VU046974.D
Acq On : 01 Feb 2022 19:28
Operator : SY/MD
Sample : N1273-21 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020122\
Data File : VU046974.D
Acq On : 01 Feb 2022 19:28
Operator : SY/MD
Sample : N1273-21 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc