

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020122\
 Data File : VU046988.D
 Acq On : 02 Feb 2022 01:47
 Operator : SY/MD
 Sample : N1349-14 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HQ3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU046988.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	98	rVB	65122	75653	5.60%	1.362%
2	1.922	171	181	204	rBV	47800	65545	4.85%	1.180%
3	2.585	371	387	406	rBV4	204084	396827	29.35%	7.146%
4	4.665	1012	1034	1075	rBV4	68916	265621	19.64%	4.783%
5	5.067	1144	1159	1190	rVB	77077	173011	12.80%	3.116%
6	5.317	1224	1237	1253	rBV2	18376	41196	3.05%	0.742%
7	5.729	1345	1365	1386	rBV2	149006	391614	28.96%	7.052%
8	6.253	1515	1528	1544	rBV	115641	220145	16.28%	3.965%
9	6.546	1604	1619	1639	rBV	725418	1352151	100.00%	24.350%
10	6.694	1652	1665	1687	rVB	95483	193493	14.31%	3.485%
11	7.568	1923	1937	1954	rBV	43396	75957	5.62%	1.368%
12	7.899	2028	2040	2062	rBV	153123	287107	21.23%	5.170%
13	8.182	2116	2128	2142	rBV2	27615	46713	3.45%	0.841%
14	8.555	2230	2244	2259	rBV2	286808	503066	37.20%	9.060%
15	8.636	2259	2269	2312	rVB	250325	479297	35.45%	8.631%
16	9.420	2499	2513	2534	rBV	194006	333885	24.69%	6.013%
17	10.758	2917	2929	2944	rBV	80530	128831	9.53%	2.320%
18	11.812	3245	3257	3272	rBV	181975	283994	21.00%	5.114%
19	12.195	3363	3376	3391	rBV	149436	238791	17.66%	4.300%




Sum of corrected areas: 5552897

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020122\
Data File : VU046988.D
Acq On : 02 Feb 2022 01:47
Operator : SY/MD
Sample : N1349-14 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

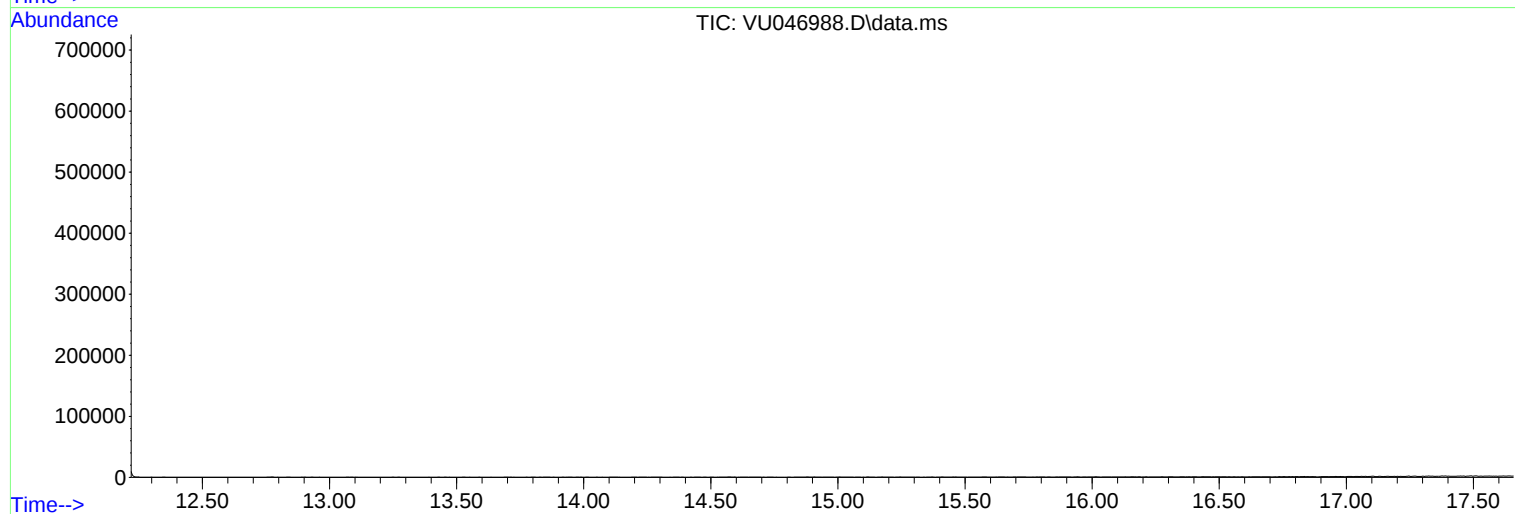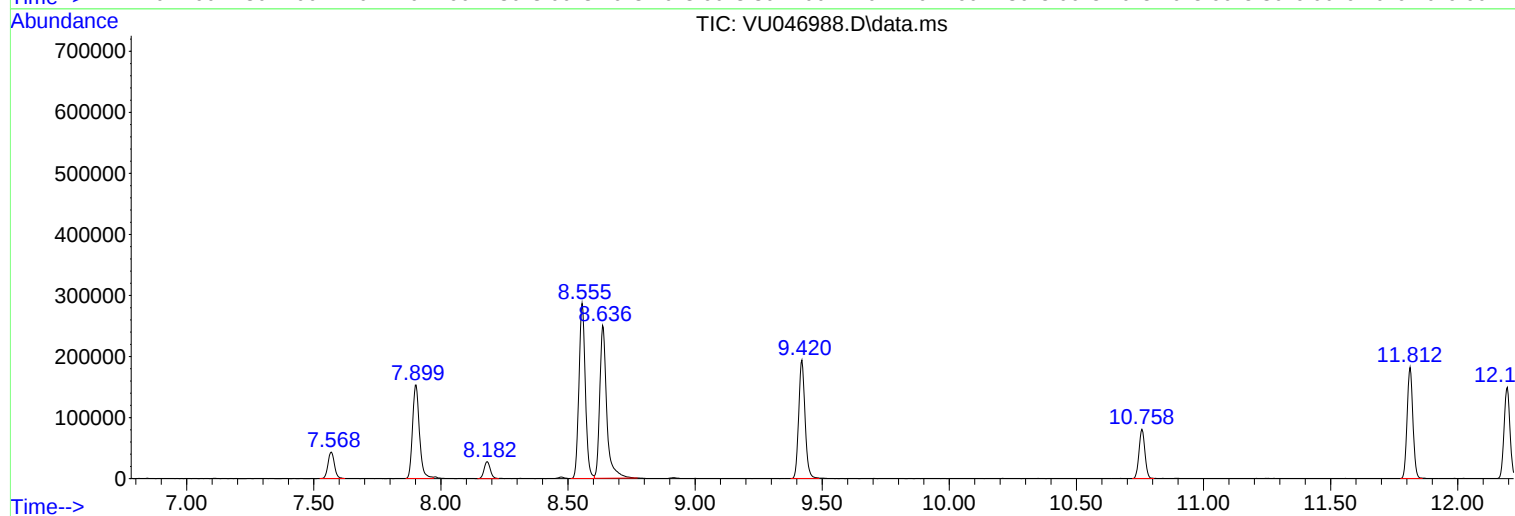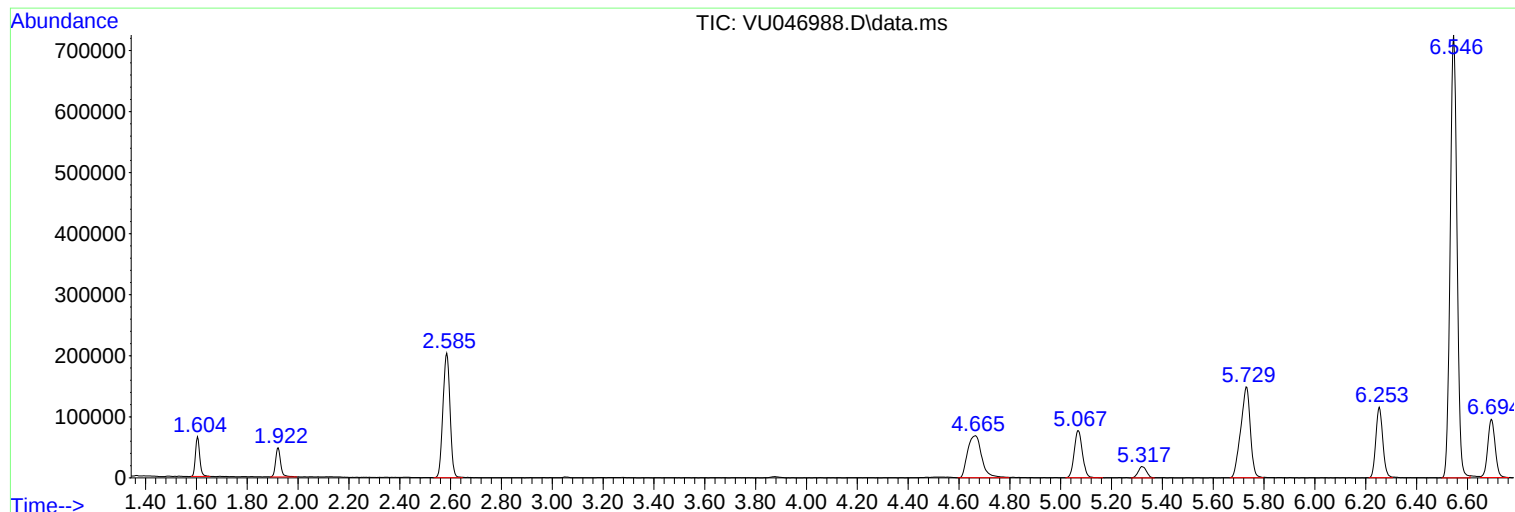

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020122\
Data File : VU046988.D
Acq On : 02 Feb 2022 01:47
Operator : SY/MD
Sample : N1349-14 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020122\
Data File : VU046988.D
Acq On : 02 Feb 2022 01:47
Operator : SY/MD
Sample : N1349-14 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
