
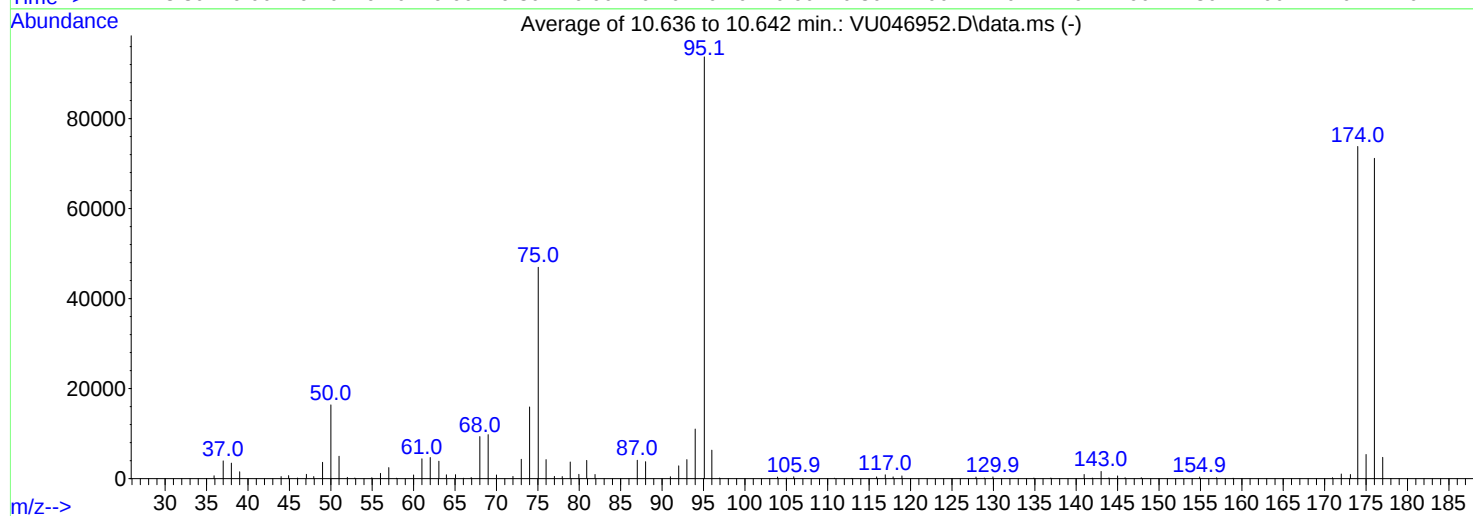


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020122\
 Data File : VU046952.D
 Acq On : 01 Feb 2022 08:54
 Operator : SY/MD
 Sample : BFB051
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB051

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 03 06:20:22 2022

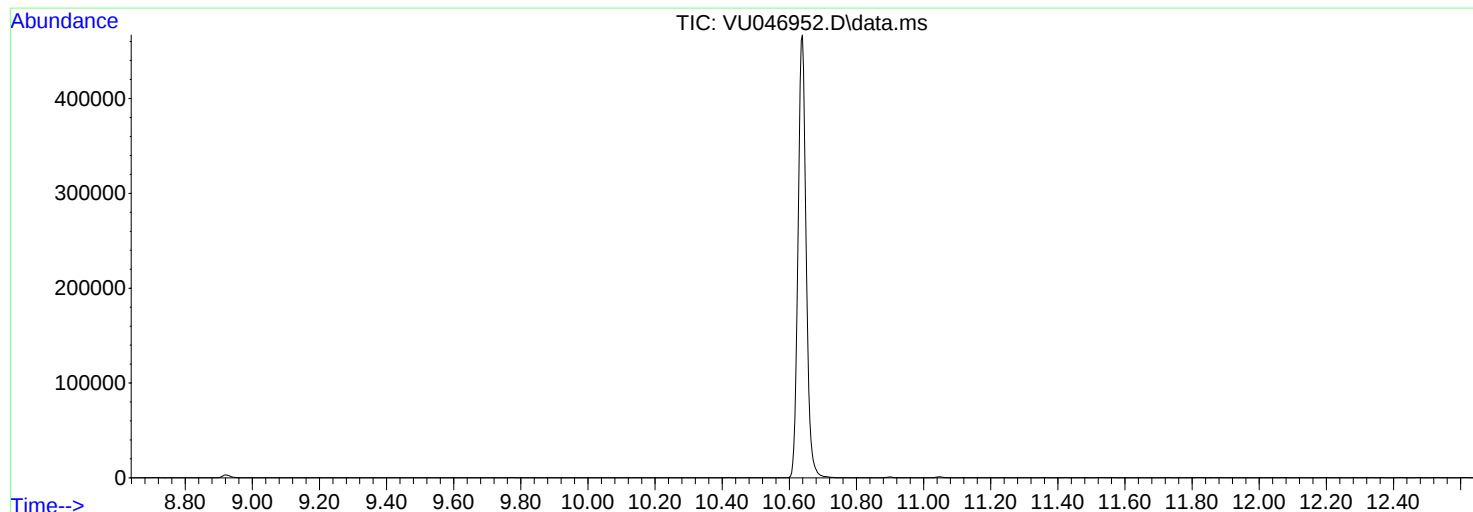

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	16389	PASS
75	95	30	60	50.1	46944	PASS
95	95	100	100	100.0	93715	PASS
96	95	5	9	6.8	6340	PASS
173	174	0.00	2	1.2	916	PASS
174	95	50	100	78.7	73787	PASS
175	174	5	9	7.3	5359	PASS
176	174	95	101	96.4	71165	PASS
177	176	5	9	6.6	4728	PASS

m/z	Abundance
44.00	192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB051

m/z	Abundance
35.90	656.0
37.00	4103.0
38.00	3459.0
39.00	1615.0
44.00	666.0
44.90	673.0
46.00	110.0
47.00	1011.0
48.00	479.0
49.00	3765.0
50.00	16920.0
51.00	5144.0
52.00	267.0
53.00	143.0
55.00	216.0
56.00	1289.0
57.00	2459.0
57.90	100.0
60.00	881.0
61.00	4727.0
62.00	4820.0
63.00	4081.0
64.00	904.0
65.10	917.0
66.00	121.0
67.00	266.0
68.00	9663.0
69.00	9870.0
70.00	825.0
72.00	534.0
73.00	4306.0
74.00	16062.0
75.00	48480.0
76.00	4399.0
77.00	484.0
78.00	444.0
78.90	3836.0
80.00	927.0
80.90	4255.0
81.90	971.0
87.00	4166.0
88.00	3772.0
91.00	425.0
92.00	3044.0
93.00	4149.0
94.00	11284.0
95.10	96552.0
96.00	6526.0
96.90	139.0
103.90	357.0
105.00	128.0
105.90	465.0
110.80	135.0
112.90	109.0
115.90	368.0
116.90	818.0
117.90	379.0
119.00	615.0
127.90	384.0
128.90	148.0
130.00	459.0
135.00	177.0
136.90	144.0
140.90	913.0
141.90	123.0
143.00	1608.0
144.00	173.0
145.00	644.0
145.90	221.0
147.80	224.0
154.90	336.0
157.00	175.0
159.00	128.0
170.90	267.0
172.00	1013.0
173.10	931.0
174.00	73704.0
175.00	5229.0
176.00	71000.0
177.00	4697.0
178.00	131.0

Instrument :
MSVOA_U
ClientSampleId :
BFB051

m/z	Abundance
35.90	668.0
37.00	4170.0
38.00	3552.0
39.00	1567.0
44.00	674.0
44.90	680.0
46.00	139.0
47.10	978.0
47.90	499.0
49.00	3731.0
50.00	16904.0
51.00	5083.0
52.00	305.0
52.90	150.0
54.90	201.0
56.00	1215.0
57.00	2561.0
58.00	120.0
60.00	860.0
61.00	4516.0
62.00	4826.0
63.00	3937.0
64.00	867.0
65.10	899.0
66.10	135.0
66.90	265.0
68.00	9588.0
69.00	10119.0
70.00	844.0
72.00	524.0
73.00	4434.0
74.00	16384.0
75.00	48400.0
76.00	4359.0
77.00	523.0
77.90	471.0
78.90	3766.0
79.90	987.0
80.90	4236.0
81.90	947.0
87.00	4198.0
88.00	3873.0
91.00	463.0
92.00	2919.0
93.00	4325.0
94.00	11407.0
95.10	96568.0
96.00	6502.0
97.00	153.0
103.90	363.0
105.00	130.0
105.90	450.0
110.80	127.0
112.90	110.0
115.90	394.0
117.00	905.0
117.90	397.0
118.90	610.0
127.90	369.0
128.90	161.0
129.90	407.0
134.90	146.0
136.90	138.0
140.90	954.0
142.00	156.0
143.00	1661.0
143.90	188.0
145.00	611.0
145.90	233.0
147.90	211.0
154.90	375.0
157.00	203.0
158.90	121.0
171.00	244.0
172.00	1040.0
173.10	956.0
174.00	75896.0
175.00	5527.0
176.00	73480.0
177.00	4874.0

Instrument :
MSVOA_U
ClientSampleId :
BFB051

m/z	Abundance
35.90	600.0
37.00	3604.0
38.00	3306.0
39.00	1428.0
44.00	644.0
44.90	633.0
46.00	161.0
47.00	904.0
47.90	454.0
49.00	3366.0
50.00	15343.0
51.00	4678.0
52.00	285.0
52.80	148.0
54.90	187.0
56.00	1074.0
57.00	2348.0
58.00	111.0
60.00	768.0
61.00	4012.0
62.00	4389.0
63.10	3566.0
63.90	772.0
65.00	891.0
66.10	123.0
66.90	234.0
68.00	8802.0
69.00	9315.0
70.00	773.0
72.00	428.0
73.00	4142.0
74.00	15355.0
75.10	43952.0
76.00	3915.0
77.00	499.0
77.90	451.0
78.90	3479.0
79.90	978.0
80.90	3690.0
81.90	863.0
87.00	3896.0
88.00	3648.0
91.00	386.0
92.00	2616.0
93.00	4213.0
94.00	10363.0
95.10	88024.0
96.00	5993.0
97.00	166.0
104.00	339.0
105.00	107.0
105.90	390.0
110.80	113.0
115.90	379.0
116.90	865.0
117.90	377.0
118.90	567.0
127.90	308.0
128.90	177.0
129.90	334.0
134.80	127.0
137.00	135.0
141.00	918.0
142.00	163.0
143.00	1570.0
143.90	175.0
145.00	539.0
145.90	181.0
147.90	218.0
154.90	356.0
156.90	230.0
158.90	115.0
170.90	193.0
172.00	995.0
173.10	861.0
174.00	71760.0
175.00	5322.0
176.00	69016.0
177.00	4613.0

Instrument :
MSVOA_U
ClientSampleId :
BFB051