

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020322\
 Data File : VU047027.D
 Acq On : 03 Feb 2022 17:26
 Operator : SY/MD
 Sample : N1328-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU047027.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	94	rVB	54395	61410	15.30%	1.985%
2	1.916	170	179	195	rBV	45557	61722	15.37%	1.995%
3	2.572	371	383	398	rVB	82429	134715	33.56%	4.355%
4	4.629	1010	1023	1053	rBV	62666	158310	39.43%	5.118%
5	5.067	1143	1159	1181	rBV	77079	172152	42.88%	5.565%
6	5.729	1344	1365	1386	rBV2	139250	367610	91.57%	11.883%
7	6.253	1514	1528	1548	rBV	108719	210192	52.36%	6.795%
8	6.694	1651	1665	1684	rBV2	90696	178172	44.38%	5.760%
9	7.568	1923	1937	1950	rBV2	39349	68147	16.97%	2.203%
10	7.903	2028	2041	2060	rBV	137410	258574	64.41%	8.359%
11	8.182	2117	2128	2141	rBV2	25765	42320	10.54%	1.368%
12	8.475	2208	2219	2232	rBV2	8802	14960	3.73%	0.484%
13	8.555	2237	2244	2253	rVB6	4162	6543	1.63%	0.212%
14	8.636	2256	2269	2311	rBV	205970	401471	100.00%	12.978%
15	9.420	2500	2513	2536	rBV	178114	317466	79.08%	10.262%
16	10.758	2916	2929	2944	rVB	75874	119907	29.87%	3.876%
17	10.896	2961	2972	2983	rBV2	8978	14724	3.67%	0.476%
18	11.812	3245	3257	3275	rVB	171616	273444	68.11%	8.839%
19	12.195	3364	3376	3393	rVB	142473	231652	57.70%	7.488%




Sum of corrected areas: 3093491

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020322\
Data File : VU047027.D
Acq On : 03 Feb 2022 17:26
Operator : SY/MD
Sample : N1328-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

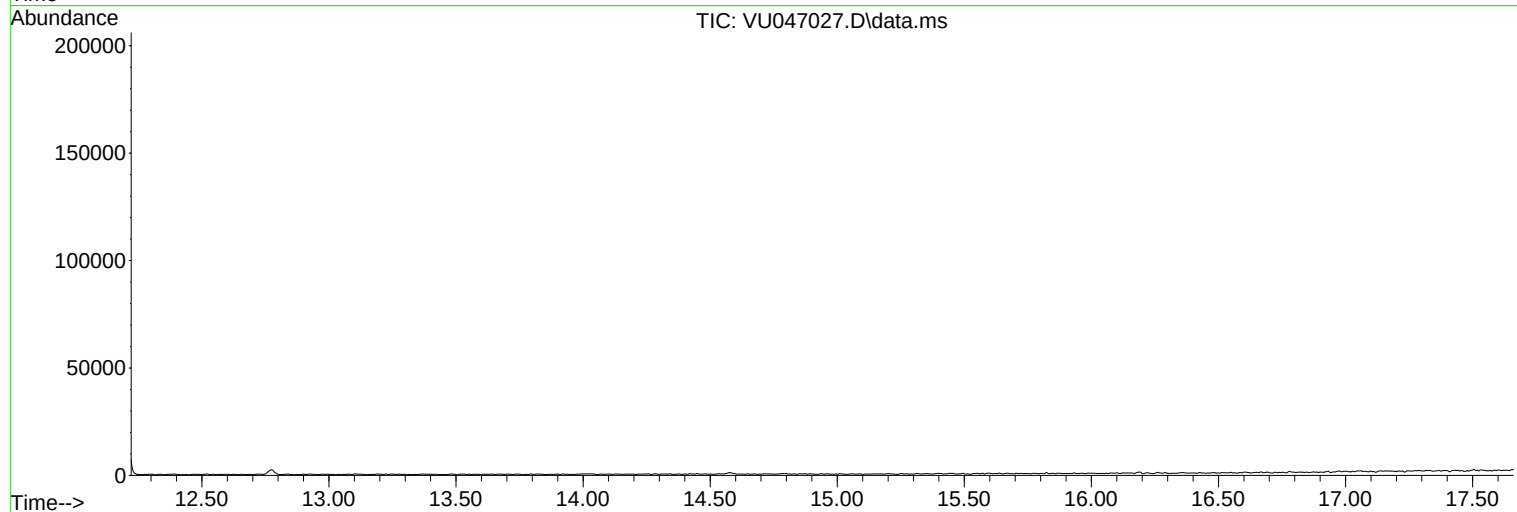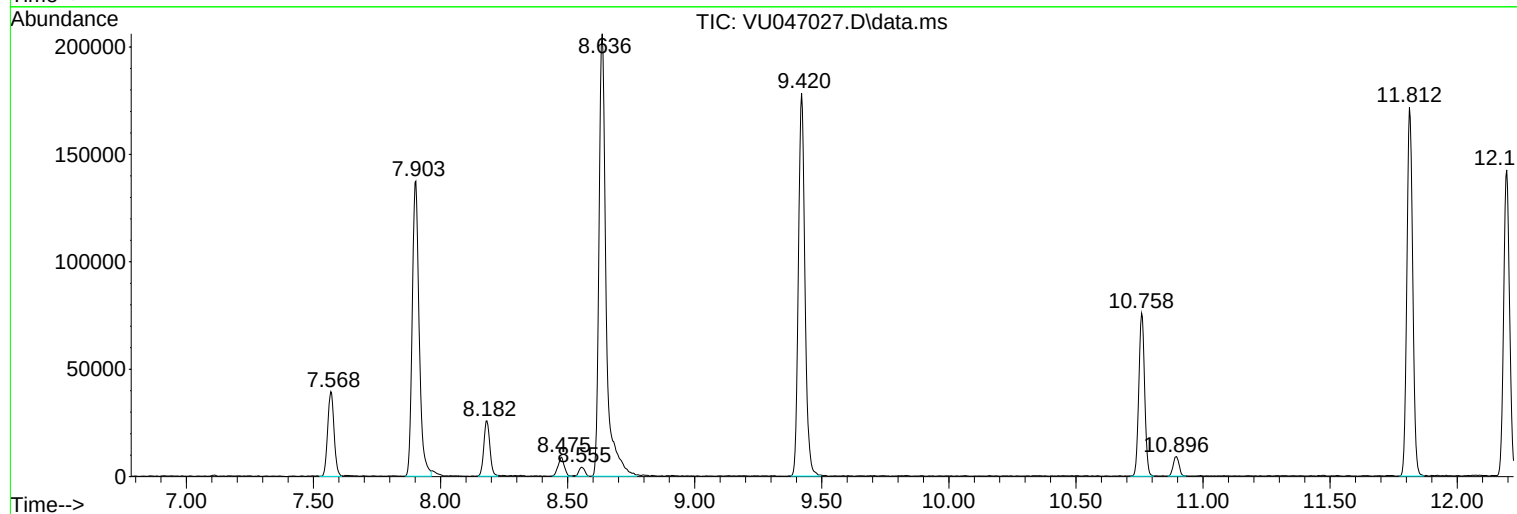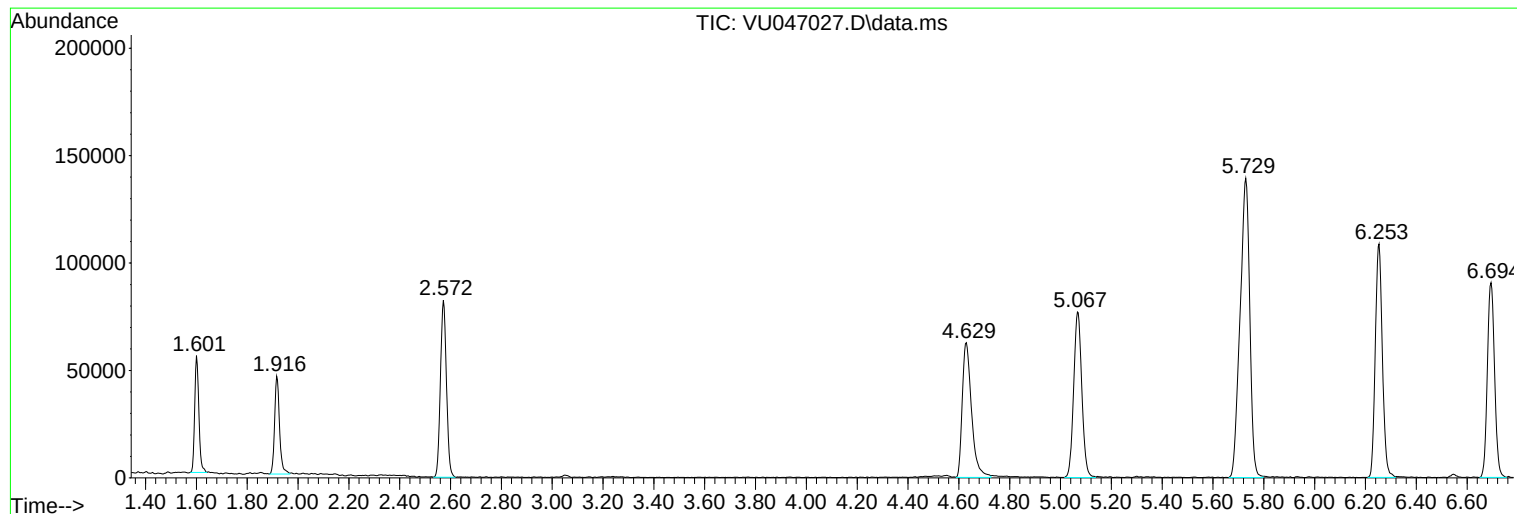

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020322\
Data File : VU047027.D
Acq On : 03 Feb 2022 17:26
Operator : SY/MD
Sample : N1328-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020322\
Data File : VU047027.D
Acq On : 03 Feb 2022 17:26
Operator : SY/MD
Sample : N1328-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc