

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020322\
 Data File : VU047034.D
 Acq On : 03 Feb 2022 20:15
 Operator : SY/MD
 Sample : N1349-02DL 4000X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HP1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU047034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	93	rBV	54518	62540	15.01%	1.753%
2	1.919	170	180	200	rBV	43989	61037	14.65%	1.711%
3	2.572	372	383	400	rVB2	91030	155556	37.33%	4.361%
4	4.633	1010	1024	1046	rBV	65145	164468	39.47%	4.611%
5	5.067	1143	1159	1181	rBV	78883	173041	41.52%	4.851%
6	5.321	1225	1238	1255	rVB6	3229	7922	1.90%	0.222%
7	5.729	1344	1365	1390	rBV2	144824	379190	90.99%	10.631%
8	6.253	1511	1528	1545	rBV	124984	238206	57.16%	6.678%
9	6.546	1606	1619	1639	rBV	124483	232176	55.72%	6.509%
10	6.694	1651	1665	1685	rVB2	96382	185540	44.52%	5.202%
11	7.568	1923	1937	1954	rBV	42451	73649	17.67%	2.065%
12	7.899	2028	2040	2059	rBV	146337	269268	64.62%	7.549%
13	8.179	2113	2127	2142	rBV2	26681	44208	10.61%	1.239%
14	8.472	2210	2218	2230	rBV2	3606	5789	1.39%	0.162%
15	8.555	2233	2244	2256	rVB2	35931	61434	14.74%	1.722%
16	8.636	2256	2269	2304	rBV	223910	416716	100.00%	11.683%
17	9.420	2500	2513	2541	rBV	205298	353486	84.83%	9.910%
18	10.758	2917	2929	2945	rBV	76890	124291	29.83%	3.484%
19	11.812	3243	3257	3273	rBV	196420	314343	75.43%	8.813%
20	12.195	3364	3376	3391	rBV	149057	244126	58.58%	6.844%




Sum of corrected areas: 3566986

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020322\
Data File : VU047034.D
Acq On : 03 Feb 2022 20:15
Operator : SY/MD
Sample : N1349-02DL 4000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HP1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

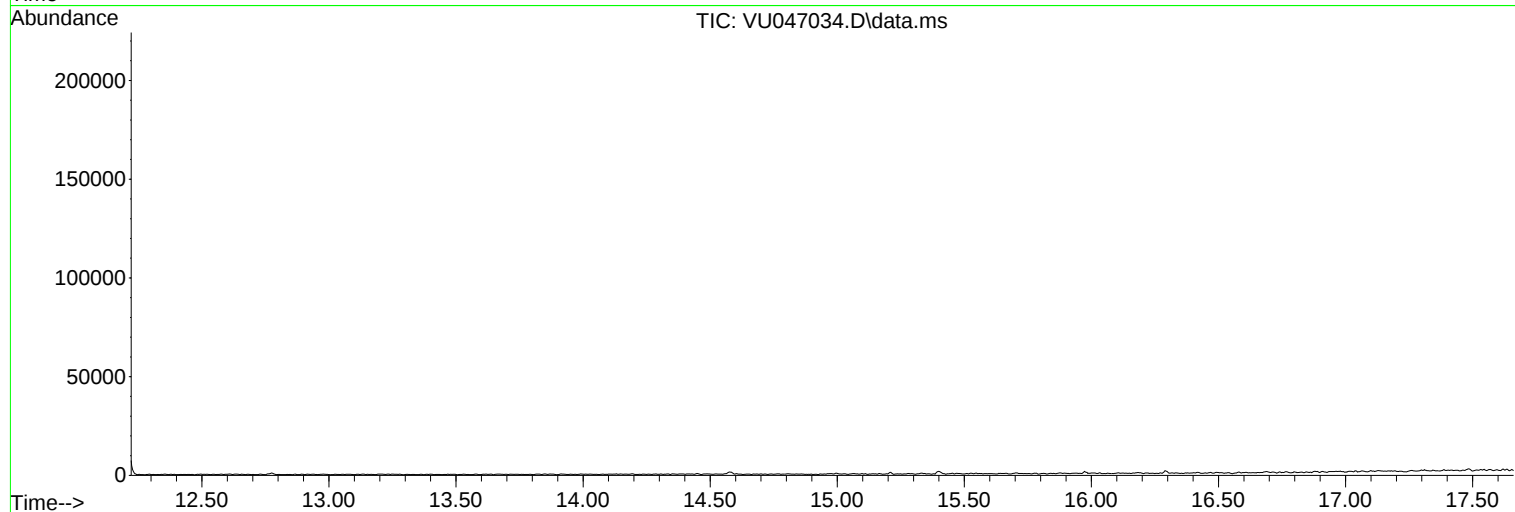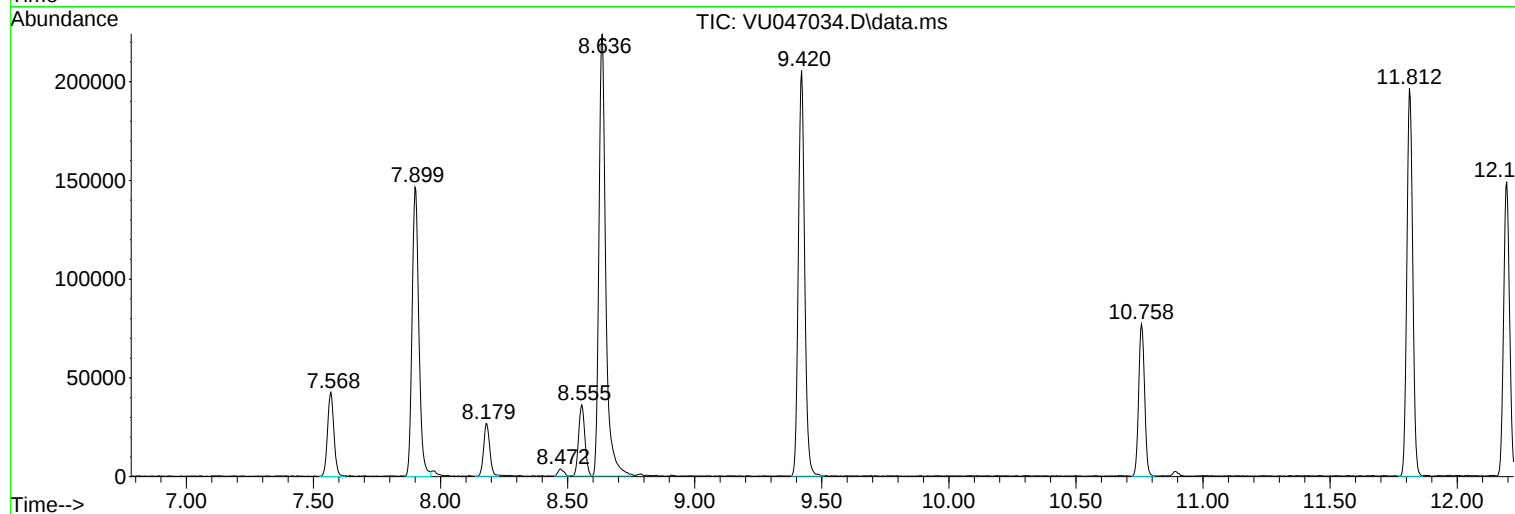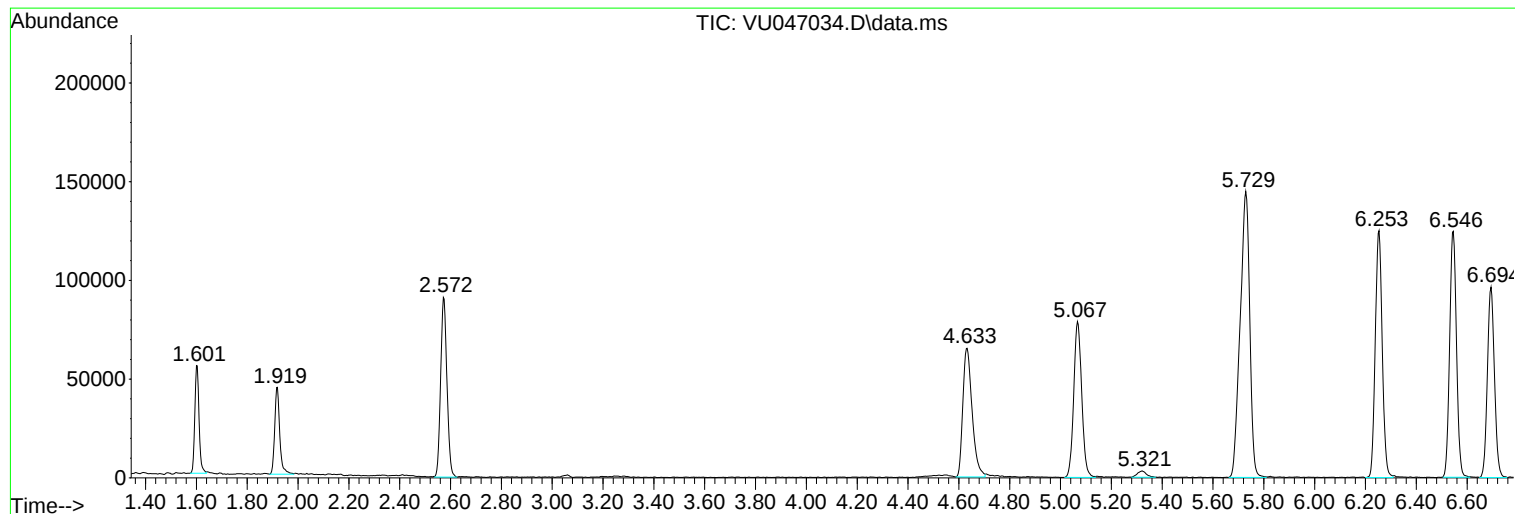

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020322\
Data File : VU047034.D
Acq On : 03 Feb 2022 20:15
Operator : SY/MD
Sample : N1349-02DL 4000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HP1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020322\
Data File : VU047034.D
Acq On : 03 Feb 2022 20:15
Operator : SY/MD
Sample : N1349-02DL 4000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HP1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc