

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020322\
 Data File : VU047035.D
 Acq On : 03 Feb 2022 20:39
 Operator : SY/MD
 Sample : N1349-03DL 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HP2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047035.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	97	rBV	52019	60493	14.76%	1.743%
2	1.919	170	180	192	rBV	42717	58035	14.16%	1.673%
3	2.572	371	383	396	rBV	82842	134355	32.78%	3.872%
4	3.195	564	577	585	rBV3	2023	4154	1.01%	0.120%
5	4.633	1010	1024	1049	rBV	66813	185379	45.23%	5.342%
6	5.067	1144	1159	1177	rBV	76752	167283	40.82%	4.821%
7	5.729	1344	1365	1384	rBV2	139874	366970	89.54%	10.576%
8	6.253	1514	1528	1552	rBV	122885	236308	57.66%	6.810%
9	6.546	1610	1619	1628	rVB4	3029	4992	1.22%	0.144%
10	6.694	1652	1665	1680	rBV	92045	178387	43.53%	5.141%
11	7.568	1926	1937	1950	rBV2	41337	70668	17.24%	2.037%
12	7.899	2028	2040	2059	rBV	139739	257228	62.77%	7.413%
13	8.182	2114	2128	2143	rBV	25866	44208	10.79%	1.274%
14	8.475	2208	2219	2229	rVB	2997	5075	1.24%	0.146%
15	8.555	2230	2244	2258	rBV2	147432	257000	62.71%	7.407%
16	8.636	2258	2269	2304	rVB	223764	409819	100.00%	11.811%
17	9.420	2498	2513	2530	rBV	201624	351135	85.68%	10.119%
18	10.758	2917	2929	2943	rBV	77943	124361	30.35%	3.584%
19	10.896	2961	2972	2982	rBV4	3365	5310	1.30%	0.153%
20	11.812	3244	3257	3274	rBV	196728	311390	75.98%	8.974%
21	12.195	3364	3376	3391	rBV	147205	237347	57.92%	6.840%




Sum of corrected areas: 3469897

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020322\
Data File : VU047035.D
Acq On : 03 Feb 2022 20:39
Operator : SY/MD
Sample : N1349-03DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HP2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

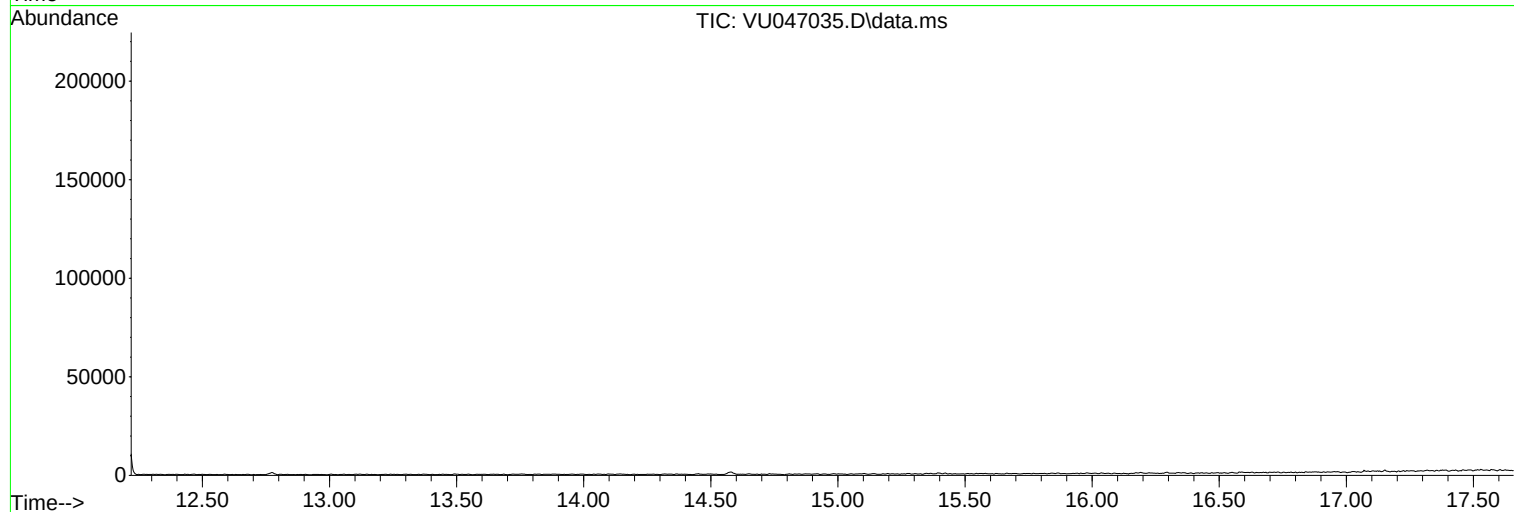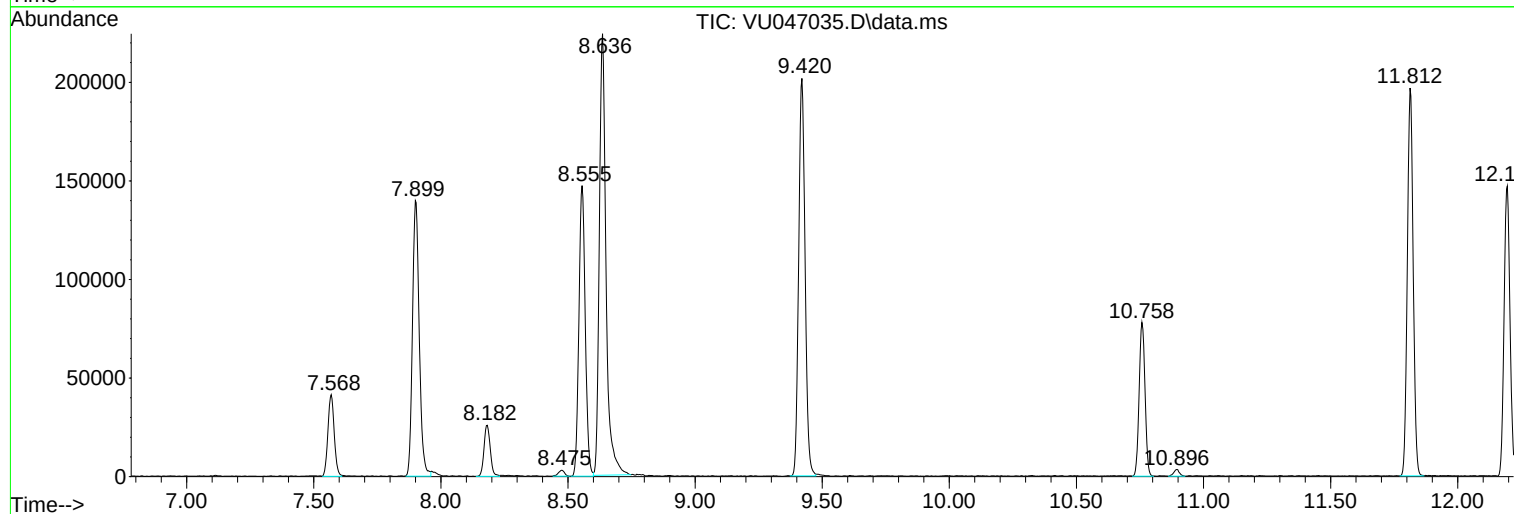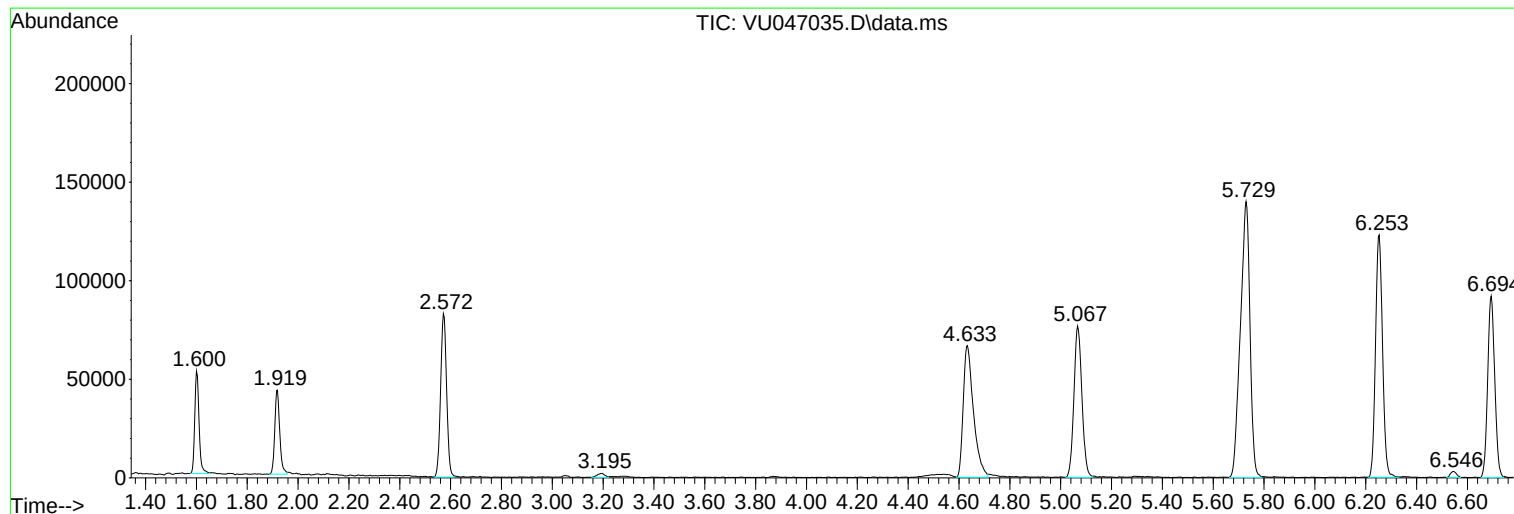

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020322\
Data File : VU047035.D
Acq On : 03 Feb 2022 20:39
Operator : SY/MD
Sample : N1349-03DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HP2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020322\
Data File : VU047035.D
Acq On : 03 Feb 2022 20:39
Operator : SY/MD
Sample : N1349-03DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HP2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc