
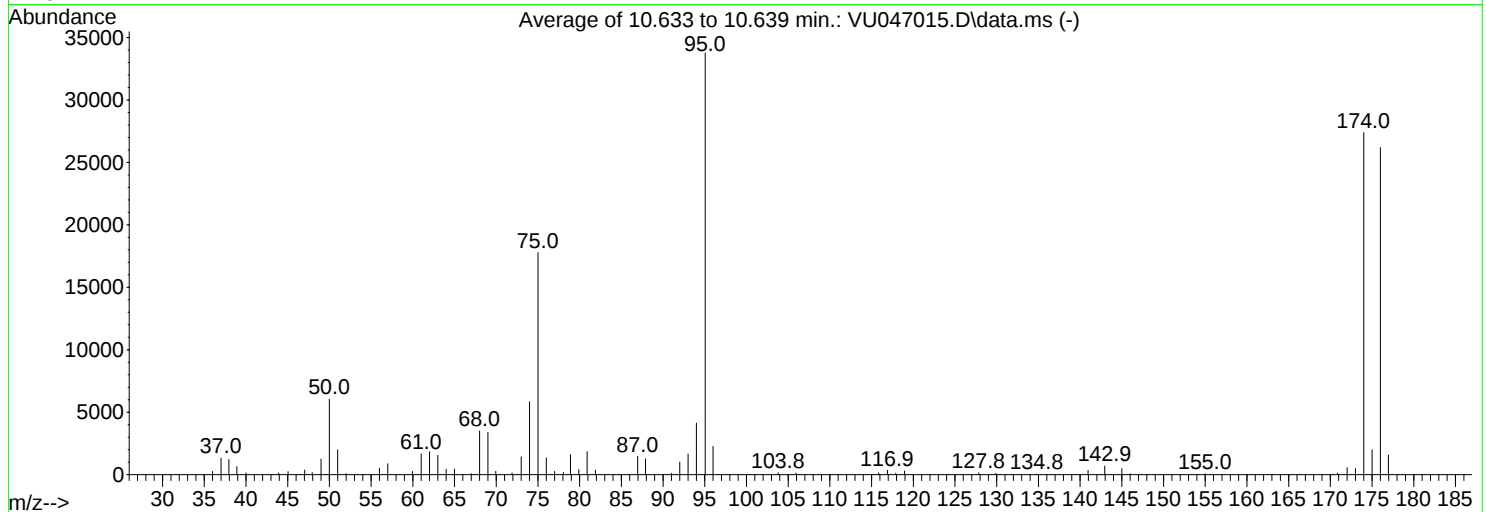


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020322\
 Data File : VU047015.D
 Acq On : 03 Feb 2022 10:43
 Operator : SY/MD
 Sample : BFB053
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB053

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Feb 03 02:56:36 2022

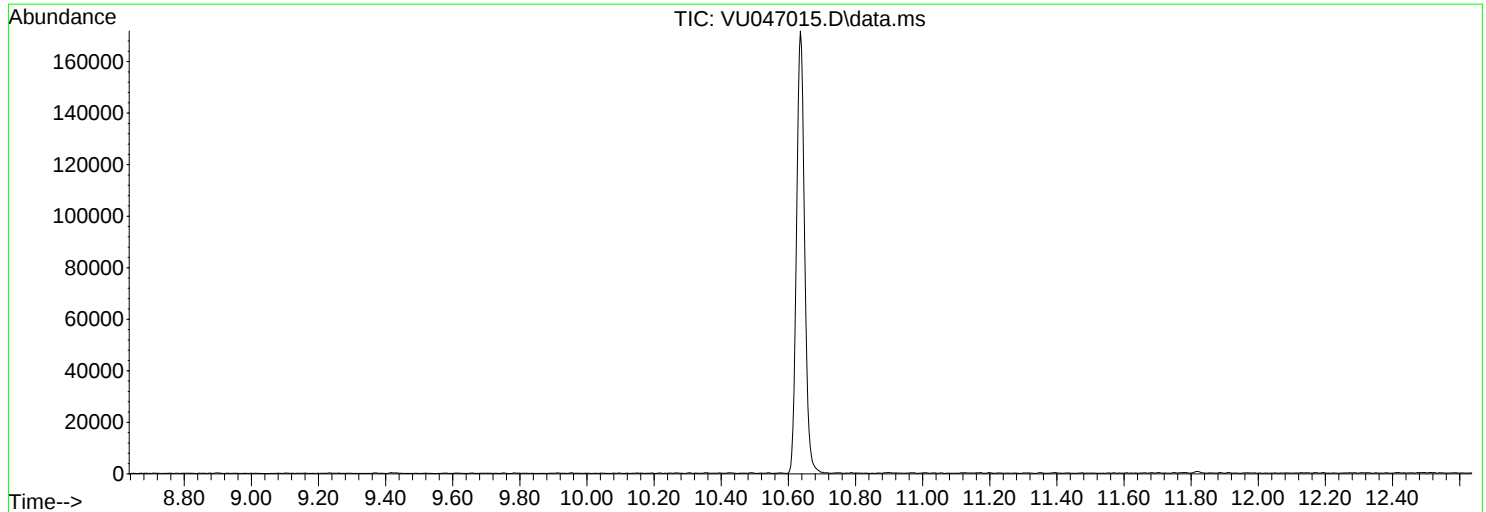

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	6037	PASS
75	95	30	80	52.6	17781	PASS
95	95	100	100	100.0	33776	PASS
96	95	5	9	6.7	2264	PASS
173	174	0.00	2	1.8	487	PASS
174	95	50	120	81.1	27397	PASS
175	174	5	9	7.3	1988	PASS
176	174	95	101	95.6	26189	PASS
177	176	5	9	6.0	1578	PASS

m/z	Abundance
43.90	214.0

Instrument :
MSVOA_U
ClientSampleId :
BFB053

m/z	Abundance
36.00	271.0
37.00	1366.0
37.90	1229.0
38.90	652.0
39.90	133.0
44.00	332.0
45.00	298.0
47.10	363.0
47.90	162.0
49.00	1338.0
50.00	6035.0
51.00	2057.0
52.00	149.0
56.00	468.0
57.00	889.0
60.00	261.0
61.00	1728.0
62.00	1857.0
63.00	1495.0
64.00	431.0
65.00	427.0
67.00	100.0
68.00	3492.0
69.00	3547.0
70.00	284.0
71.90	139.0
73.00	1450.0
74.00	5827.0
75.00	17384.0
76.00	1411.0
77.00	257.0
78.00	183.0
78.90	1631.0
79.90	387.0
80.90	1802.0
81.90	359.0
87.00	1583.0
87.90	1361.0
92.00	1036.0
93.00	1612.0
94.00	4019.0
95.00	33392.0
96.00	2358.0
103.80	165.0
105.90	116.0
115.80	125.0
116.90	341.0
117.90	108.0
118.90	320.0
127.90	132.0
141.00	348.0
142.90	628.0
145.00	465.0
170.90	113.0
172.00	566.0
173.00	423.0
174.00	26440.0
175.00	1914.0
176.00	25208.0
177.00	1508.0

Instrument :
MSVOA_U
ClientSampleId :
BFB053

m/z	Abundance
36.00	261.0
37.00	1332.0
38.00	1233.0
38.90	673.0
40.00	140.0
44.00	334.0
45.00	241.0
47.00	410.0
48.00	173.0
49.00	1271.0
50.00	6189.0
51.00	2033.0
52.00	124.0
56.00	525.0
57.00	903.0
60.00	267.0
61.00	1728.0
62.00	1860.0
63.00	1581.0
64.00	456.0
65.00	462.0
67.00	121.0
68.00	3608.0
69.00	3475.0
70.00	288.0
71.90	141.0
73.00	1445.0
74.00	6014.0
75.00	18472.0
76.00	1365.0
77.00	270.0
78.10	182.0
78.90	1621.0
79.90	409.0
80.90	1898.0
81.90	343.0
86.90	1468.0
87.90	1280.0
91.00	153.0
92.00	1033.0
93.00	1726.0
94.00	4270.0
95.10	34664.0
96.00	2306.0
103.80	163.0
106.00	127.0
115.80	143.0
116.90	334.0
117.90	128.0
118.90	306.0
127.80	158.0
129.90	135.0
141.00	352.0
143.00	721.0
145.00	503.0
146.00	121.0
155.00	102.0
170.80	112.0
172.00	559.0
173.00	503.0
174.00	28016.0
175.00	2082.0
176.00	26920.0
176.90	1592.0

Instrument :
MSVOA_U
ClientSampleId :
BFB053

m/z	Abundance
36.00	223.0
37.00	1251.0
38.00	1176.0
38.90	612.0
40.10	161.0
43.90	355.0
45.10	183.0
47.00	348.0
48.00	150.0
49.00	1129.0
50.00	5888.0
51.00	1857.0
56.00	554.0
57.00	812.0
59.90	249.0
61.00	1546.0
62.00	1766.0
63.00	1578.0
64.00	413.0
65.00	471.0
68.00	3391.0
69.00	3131.0
69.90	237.0
71.90	144.0
73.00	1368.0
74.00	5661.0
75.00	17488.0
76.00	1262.0
77.00	254.0
78.10	161.0
78.90	1548.0
79.90	439.0
80.90	1837.0
81.90	361.0
85.90	125.0
86.90	1327.0
87.90	1181.0
91.00	169.0
92.00	988.0
93.00	1633.0
94.00	4072.0
95.10	33272.0
96.00	2127.0
103.80	147.0
106.00	133.0
115.90	161.0
116.90	354.0
117.90	132.0
119.00	274.0
127.80	133.0
129.90	161.0
134.80	101.0
140.90	350.0
143.00	732.0
145.00	497.0
146.00	107.0
155.00	124.0
170.80	120.0
172.00	570.0
173.00	534.0
174.00	27736.0
175.00	1969.0
176.00	26440.0
177.00	1634.0

Instrument :
MSVOA_U
ClientSampleId :
BFB053