


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020325\
Data File : VU063108.D
Acq On : 03 Feb 2025 08:27
Operator : MD/SY
Sample : BFB071
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB071

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020325WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Feb 04 07:42:54 2025

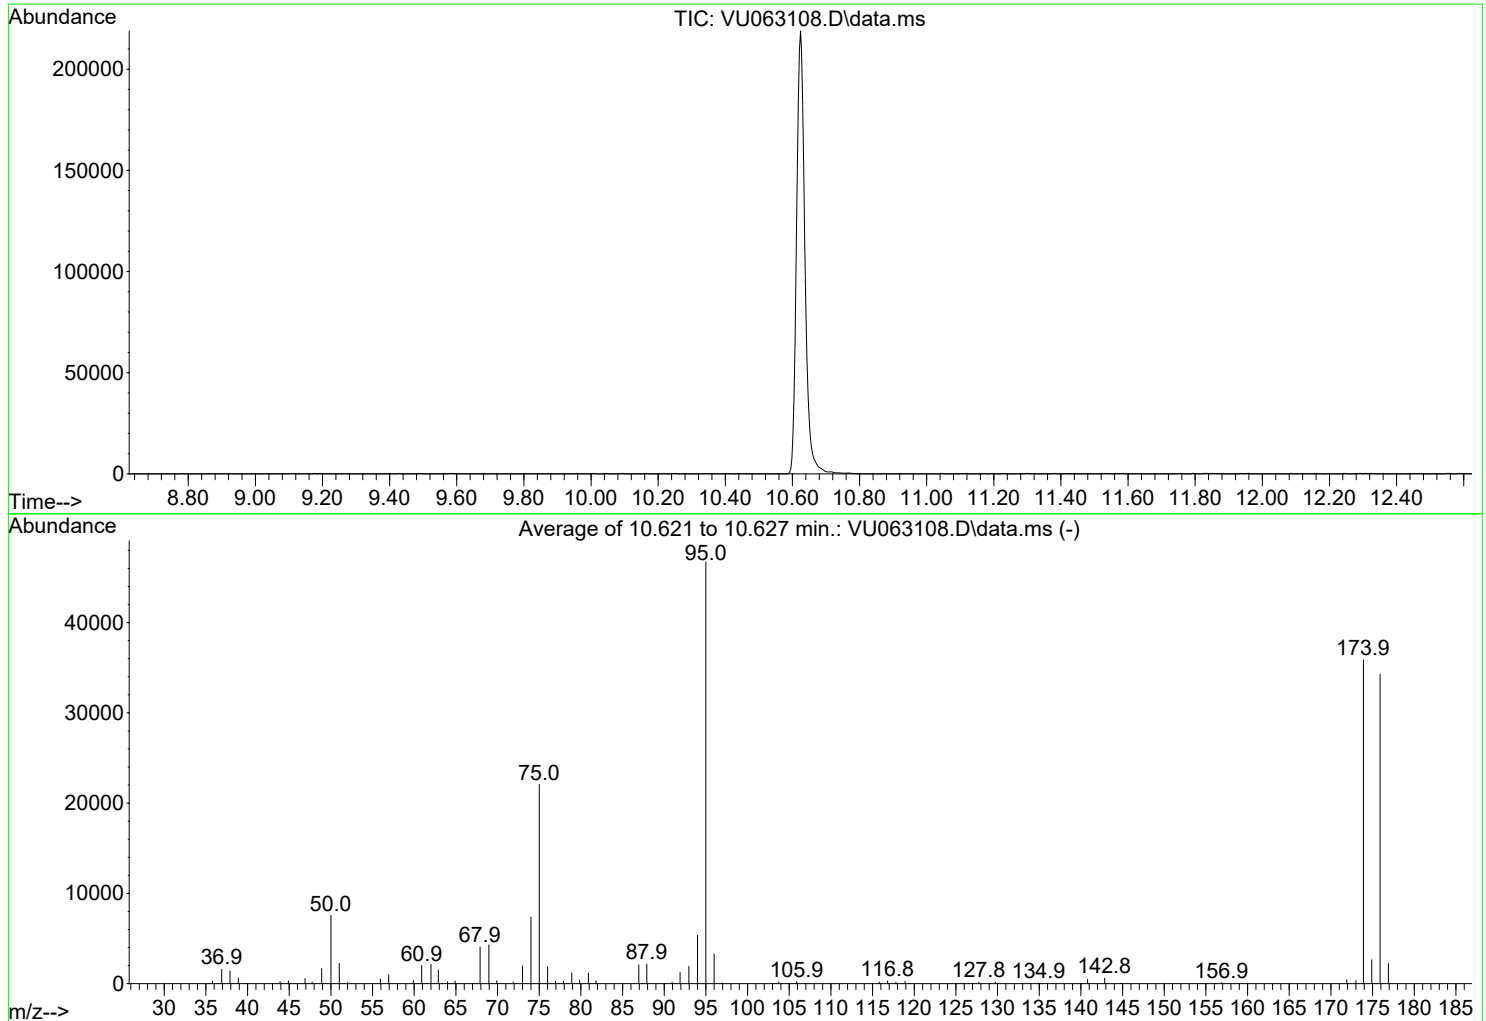

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.2	7566	PASS
75	95	30	80	47.2	22067	PASS
95	95	100	100	100.0	46731	PASS
96	95	5	9	7.0	3288	PASS
173	174	0.00	2	1.0	353	PASS
174	95	50	120	76.8	35875	PASS
175	174	5	9	7.4	2651	PASS
176	174	95	101	95.6	34285	PASS
177	176	5	9	6.5	2240	PASS

m/z Abundance

Instrument :
MSVOA_U
ClientSampleId :
BFB071

m/z	Abundance
35.80	246.0
36.90	1629.0
37.90	1430.0
38.90	617.0
39.80	110.0
43.90	261.0
44.90	324.0
46.90	517.0
47.80	193.0
48.90	1672.0
50.00	7609.0
51.00	2365.0
52.00	127.0
55.90	519.0
56.90	956.0
59.90	377.0
60.90	1946.0
62.00	2082.0
62.90	1549.0
64.00	215.0
64.90	279.0
67.90	4015.0
69.00	4269.0
69.90	353.0
71.90	170.0
73.00	2073.0
74.00	7472.0
75.00	22104.0
76.00	1953.0
77.00	278.0
77.90	261.0
78.90	1238.0
79.90	366.0
80.90	1162.0
81.80	320.0
87.00	2059.0
87.90	2153.0
91.00	141.0
91.90	1207.0
93.00	1949.0
94.00	5365.0
95.00	46248.0
96.00	3167.0
96.90	106.0
103.70	208.0
105.90	220.0
115.90	153.0
116.80	264.0
117.80	144.0
118.90	247.0
127.80	188.0
129.70	136.0
140.80	442.0
142.90	620.0
144.80	105.0
156.90	100.0
171.90	429.0
173.00	325.0
173.90	34424.0
174.90	2575.0
175.90	33368.0
176.90	2197.0

Instrument :
MSVOA_U
ClientSampleId :
BFB071

m/z	Abundance
35.90	278.0
36.90	1629.0
37.90	1431.0
38.90	670.0
43.90	245.0
44.90	308.0
46.90	596.0
47.80	189.0
48.90	1723.0
50.00	7744.0
51.00	2313.0
52.00	139.0
55.90	537.0
57.00	991.0
59.90	365.0
60.90	2086.0
62.00	2257.0
62.90	1550.0
64.00	233.0
64.90	298.0
67.90	4175.0
68.90	4384.0
69.90	320.0
71.90	181.0
73.00	2031.0
74.00	7643.0
75.00	22616.0
76.00	1929.0
76.90	265.0
77.90	243.0
78.90	1249.0
79.80	380.0
80.90	1214.0
81.80	334.0
87.00	2149.0
87.90	2276.0
90.90	160.0
91.90	1286.0
93.00	1956.0
94.00	5482.0
95.00	48240.0
96.00	3426.0
96.90	124.0
103.80	196.0
105.90	233.0
115.80	161.0
116.80	280.0
117.80	144.0
118.90	276.0
127.70	180.0
129.80	157.0
134.90	101.0
140.80	475.0
142.90	623.0
144.80	111.0
156.90	124.0
171.90	451.0
173.00	365.0
173.90	36896.0
174.90	2746.0
175.90	35360.0
176.90	2305.0

Instrument :
MSVOA_U
ClientSampleId :
BFB071

m/z	Abundance
35.90	254.0
36.90	1531.0
37.90	1352.0
38.90	646.0
43.90	211.0
44.90	265.0
46.90	569.0
47.70	160.0
48.90	1605.0
50.00	7346.0
51.00	2070.0
52.00	112.0
56.00	509.0
56.90	1003.0
59.90	322.0
60.90	2027.0
62.00	2155.0
62.90	1443.0
64.00	219.0
64.90	311.0
67.90	3984.0
69.00	4234.0
69.90	303.0
71.90	180.0
73.00	1787.0
74.00	7007.0
75.00	21480.0
76.00	1754.0
76.90	257.0
77.90	224.0
78.90	1146.0
79.90	357.0
80.90	1203.0
81.80	299.0
86.90	2035.0
87.90	2074.0
90.90	174.0
91.90	1216.0
92.90	1850.0
94.00	5293.0
95.00	45704.0
96.00	3272.0
103.80	185.0
105.90	202.0
115.70	165.0
116.80	285.0
117.80	159.0
118.90	250.0
127.70	146.0
129.80	170.0
135.00	129.0
140.80	454.0
142.80	568.0
156.90	104.0
171.90	411.0
173.00	369.0
173.90	36304.0
174.90	2632.0
175.90	34128.0
176.90	2217.0

Instrument :
MSVOA_U
ClientSampleId :
BFB071