

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020422\
 Data File : VU047052.D
 Acq On : 04 Feb 2022 17:34
 Operator : SY/MD
 Sample : N1349-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HP9

Quant Time: Feb 05 01:35:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Feb 05 01:18:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	94762	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	109101	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.815	152	49162	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	60447	4.972	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.400%
7) Chloroethane-d5	1.919	69	46152	4.918	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.400%
11) 1,1-Dichloroethene-d2	2.575	65	23337	5.363	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	107.200%
20) 2-Butanone-d5	4.629	46	123346	50.745	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.480%
24) Chloroform-d	5.070	84	98291	5.069	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.400%
26) 1,2-Dichloroethane-d4	5.706	65	50935	5.142	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.800%
32) Benzene-d6	5.732	84	195402	5.114	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.200%
36) 1,2-Dichloropropane-d6	6.693	67	60019	5.035	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.800%
41) Toluene-d8	7.902	98	156420	4.615	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.200%
43) trans-1,3-Dichloroprop...	8.182	79	22227	4.894	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.800%
46) 2-Hexanone-d5	8.635	63	101313	48.155	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.300%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	49971	4.910	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.200%
66) 1,2-Dichlorobenzene-d4	12.195	152	60345	6.029	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	120.600%#
Target Compounds						Qvalue
3) Chloromethane	1.526	50	4947	0.465	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020422\
Data File : VU047052.D
Acq On : 04 Feb 2022 17:34
Operator : SY/MD
Sample : N1349-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HP9

Quant Time: Feb 05 01:35:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Feb 05 01:18:17 2022
Response via : Initial Calibration

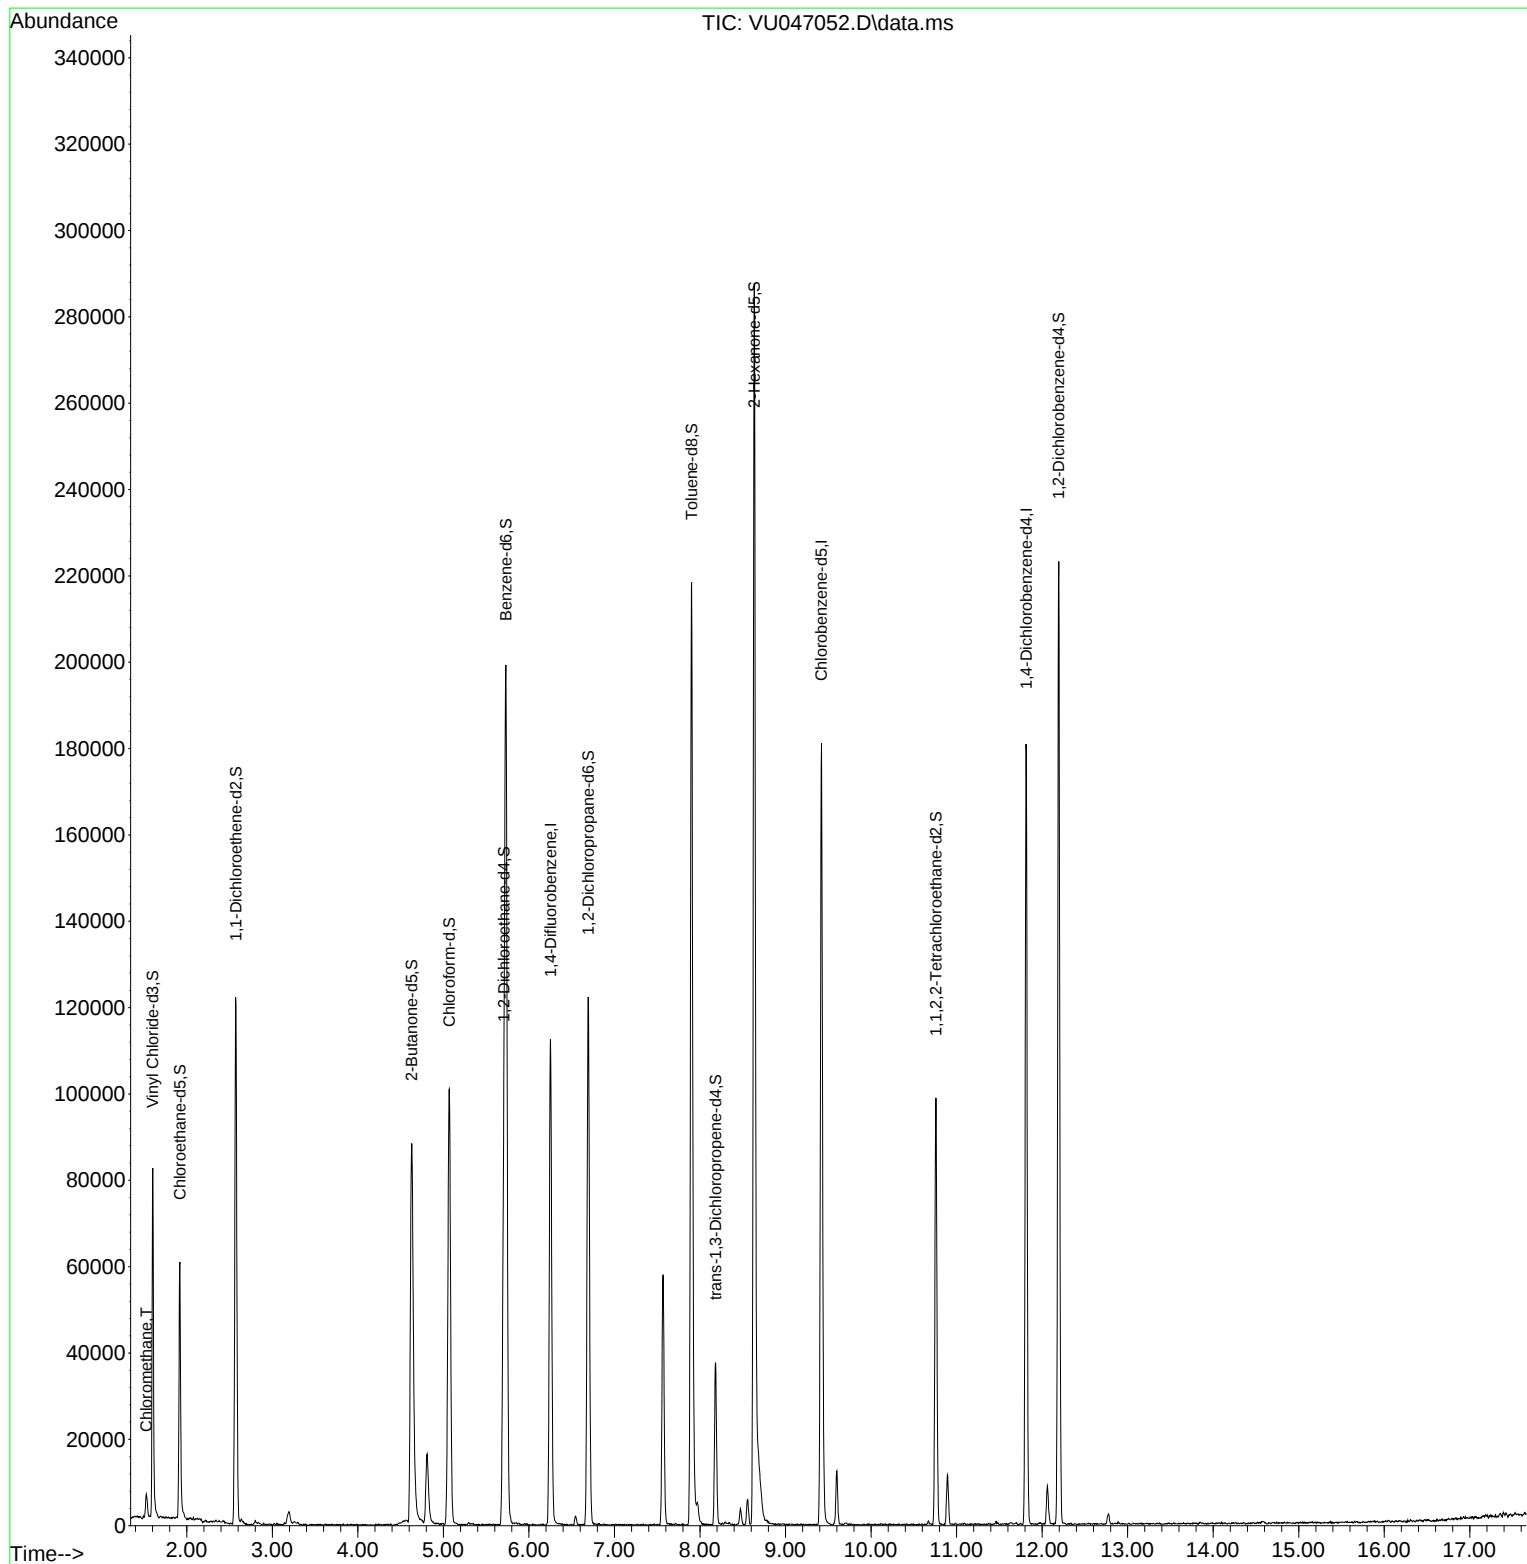

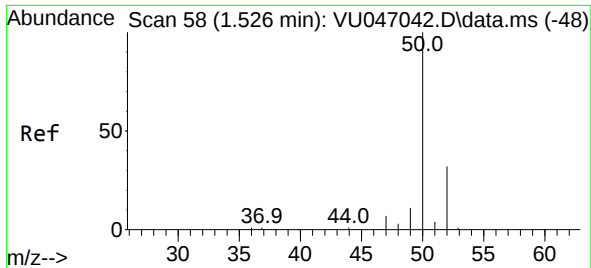

#3
 Chloromethane
 Concen: 0.465 ug/L
 RT: 1.526 min Scan# 50
 Delta R.T. -0.000 min
 Lab File: VU047052.D
 Acq: 04 Feb 2022 17:34

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HP9

Tgt Ion: 50 Resp: 4947
 Ion Ratio Lower Upper
 50 100
 52 33.9 22.7 42.3

