

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020422\
 Data File : VU047049.D
 Acq On : 04 Feb 2022 16:22
 Operator : SY/MD
 Sample : N1349-07DL 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HP6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047049.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	102	rBV	81000	95387	17.07%	1.995%
2	1.919	171	180	197	rBV	59833	80373	14.38%	1.681%
3	2.572	371	383	398	rBV2	132748	229551	41.07%	4.802%
4	4.636	1011	1025	1060	rBV2	77400	280497	50.19%	5.868%
5	5.067	1142	1159	1185	rBV	103803	230143	41.18%	4.814%
6	5.321	1224	1238	1251	rBV2	6013	12559	2.25%	0.263%
7	5.729	1343	1365	1385	rBV2	204789	530528	94.92%	11.098%
8	6.253	1513	1528	1552	rBV2	113390	219193	39.22%	4.585%
9	6.546	1607	1619	1634	rBV	55098	101581	18.18%	2.125%
10	6.694	1651	1665	1681	rBV	127079	245258	43.88%	5.130%
11	7.568	1924	1937	1953	rBV	60002	104314	18.66%	2.182%
12	7.899	2027	2040	2059	rBV	227049	413468	73.98%	8.649%
13	8.179	2117	2127	2140	rBV2	37761	62304	11.15%	1.303%
14	8.555	2231	2244	2258	rVV	280755	484950	86.77%	10.145%
15	8.636	2258	2269	2321	rVB	298814	558900	100.00%	11.691%
16	9.420	2498	2513	2533	rBV	182476	319274	57.13%	6.679%
17	10.758	2918	2929	2946	rBV	100904	161461	28.89%	3.378%
18	11.812	3246	3257	3271	rBV	184758	290807	52.03%	6.083%
19	12.195	3362	3376	3395	rBV	221803	359868	64.39%	7.528%




Sum of corrected areas: 4780416

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020422\
Data File : VU047049.D
Acq On : 04 Feb 2022 16:22
Operator : SY/MD
Sample : N1349-07DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HP6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

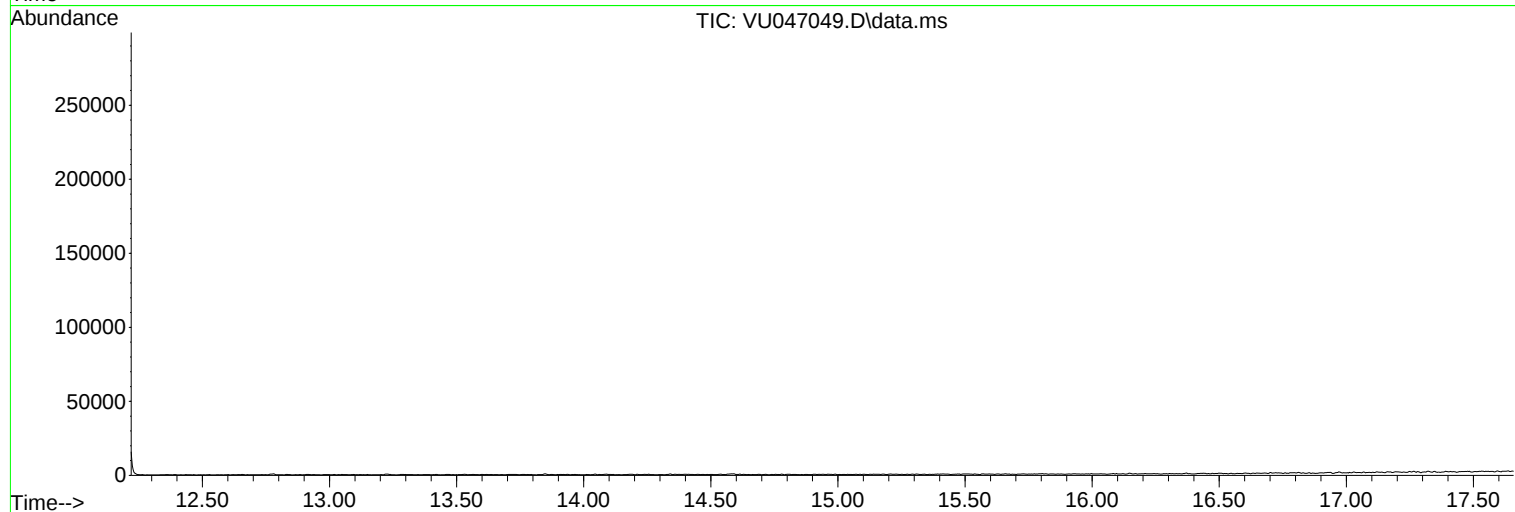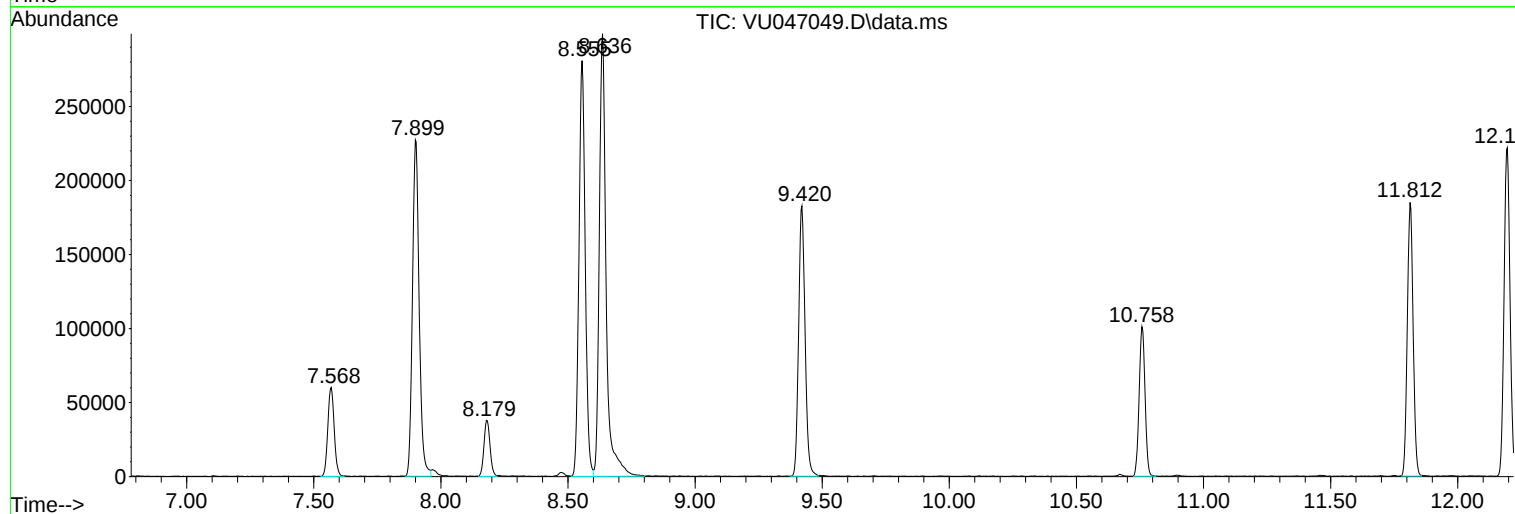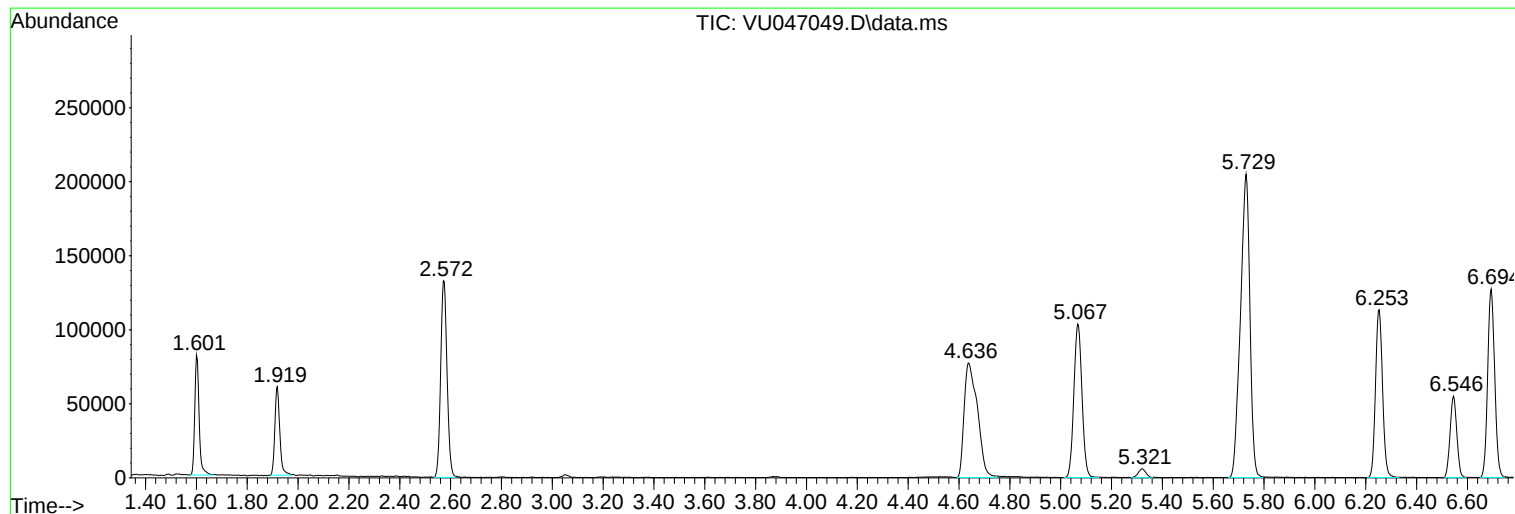

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020422\
Data File : VU047049.D
Acq On : 04 Feb 2022 16:22
Operator : SY/MD
Sample : N1349-07DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HP6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020422\
Data File : VU047049.D
Acq On : 04 Feb 2022 16:22
Operator : SY/MD
Sample : N1349-07DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HP6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc