

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020422\
 Data File : VU047050.D
 Acq On : 04 Feb 2022 16:46
 Operator : SY/MD
 Sample : N1349-14DL 500X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HQ3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047050.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	99	rVB	83201	97220	17.77%	2.185%
2	1.919	170	180	200	rBV	60421	80361	14.69%	1.806%
3	2.575	368	384	402	rBV3	138951	249207	45.56%	5.600%
4	4.633	1010	1024	1059	rBV	79911	226542	41.41%	5.091%
5	5.067	1142	1159	1177	rBV2	105128	229713	41.99%	5.162%
6	5.321	1226	1238	1249	rBV6	3666	7980	1.46%	0.179%
7	5.729	1344	1365	1389	rBV2	200832	528160	96.55%	11.869%
8	6.253	1514	1528	1550	rBV	107595	207583	37.95%	4.665%
9	6.546	1605	1619	1640	rBV	143890	268648	49.11%	6.037%
10	6.694	1648	1665	1687	rBB2	126859	243013	44.43%	5.461%
11	7.568	1924	1937	1952	rBV	58817	102437	18.73%	2.302%
12	7.899	2026	2040	2060	rBV	221264	408924	74.76%	9.190%
13	8.182	2117	2128	2141	rBV2	37927	62154	11.36%	1.397%
14	8.555	2232	2244	2257	rBV	60200	104996	19.19%	2.360%
15	8.636	2257	2269	2306	rBV	297049	547007	100.00%	12.293%
16	9.420	2497	2513	2534	rBV	174432	305671	55.88%	6.869%
17	10.758	2917	2929	2947	rVB	101011	161311	29.49%	3.625%
18	11.812	3246	3257	3273	rBV	169895	269642	49.29%	6.060%
19	12.195	3363	3376	3394	rVB	218463	349279	63.85%	7.849%




Sum of corrected areas: 4449848

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020422\
Data File : VU047050.D
Acq On : 04 Feb 2022 16:46
Operator : SY/MD
Sample : N1349-14DL 500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HQ3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

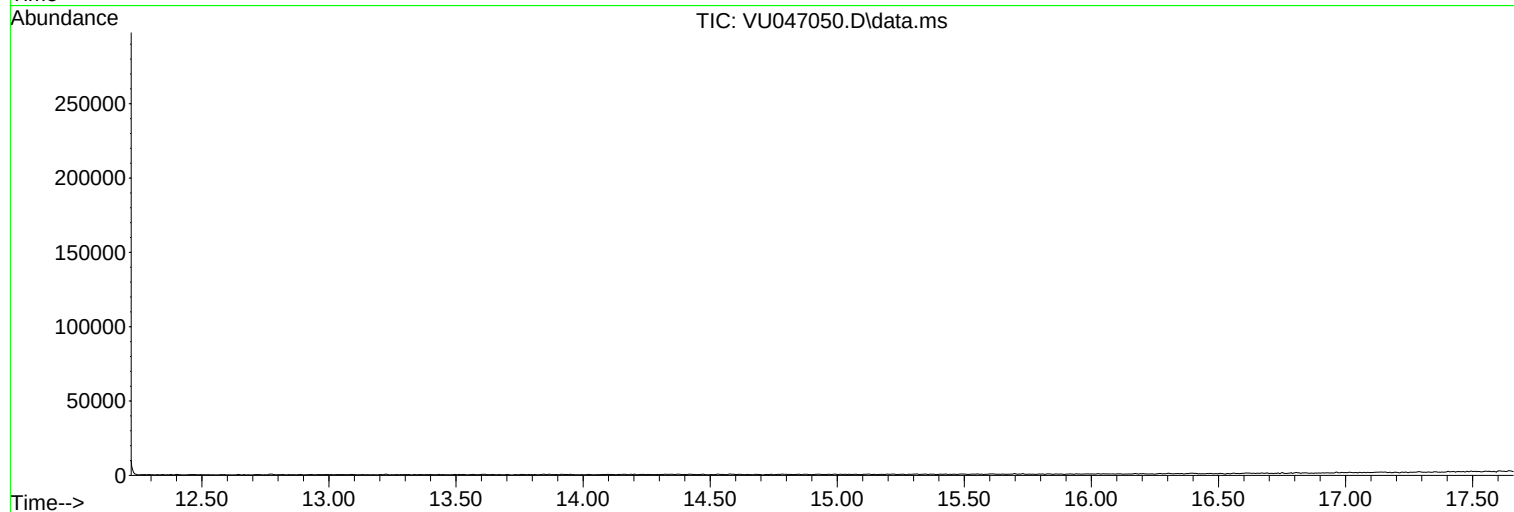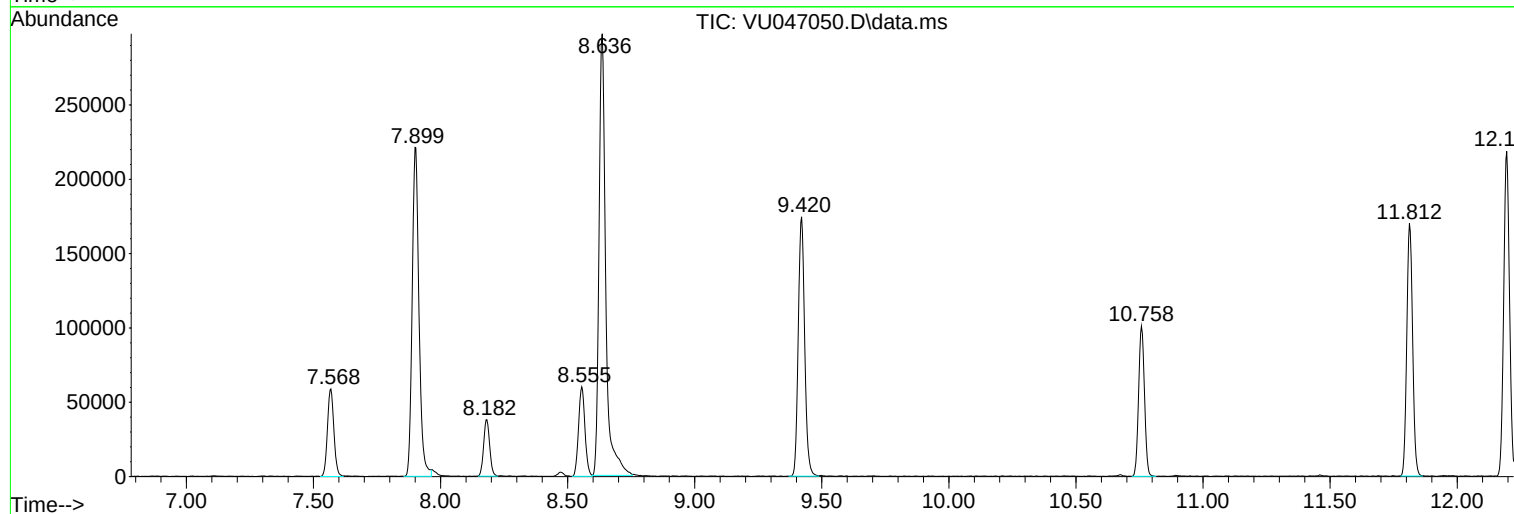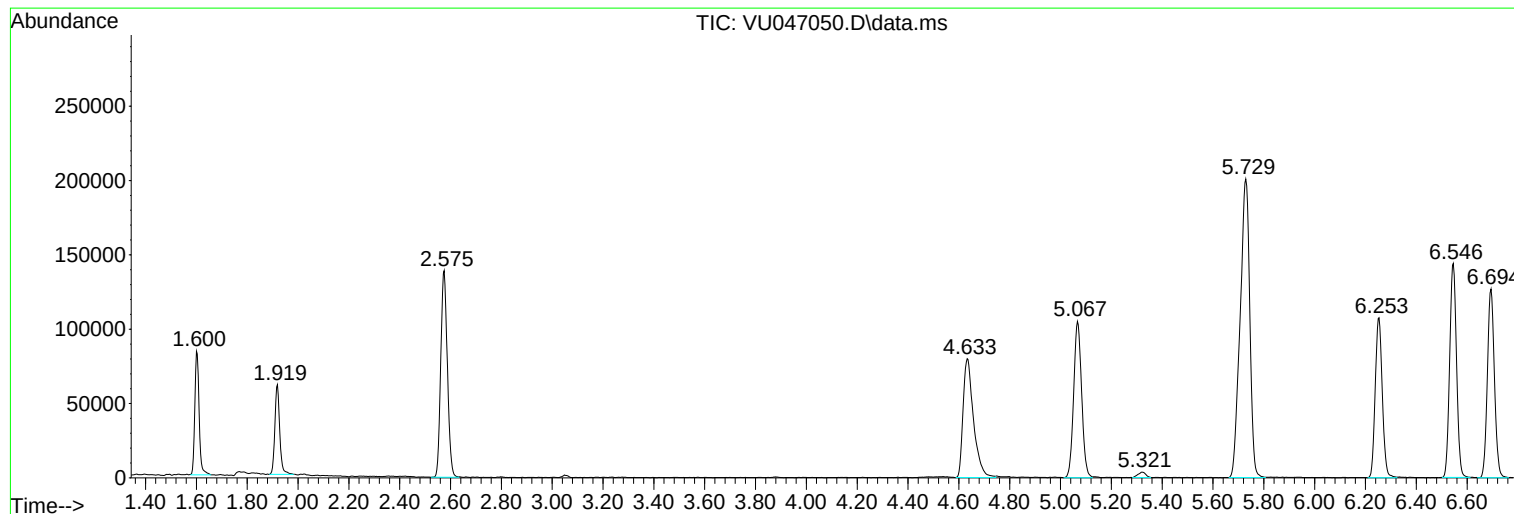

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020422\
Data File : VU047050.D
Acq On : 04 Feb 2022 16:46
Operator : SY/MD
Sample : N1349-14DL 500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HQ3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020422\
Data File : VU047050.D
Acq On : 04 Feb 2022 16:46
Operator : SY/MD
Sample : N1349-14DL 500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HQ3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc