

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020422\
 Data File : VU047054.D
 Acq On : 04 Feb 2022 18:46
 Operator : SY/MD
 Sample : VIBLK037
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK037

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047054.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	102	rVB	78747	93346	16.95%	2.136%
2	1.919	171	180	198	rBV	58819	77929	14.15%	1.783%
3	2.572	371	383	398	rBV	121653	198517	36.04%	4.543%
4	4.633	1010	1024	1061	rBV	78496	207093	37.60%	4.739%
5	5.067	1143	1159	1179	rBV	103070	224933	40.83%	5.148%
6	5.729	1343	1365	1389	rBV2	199332	519393	94.29%	11.887%
7	6.253	1510	1528	1549	rBV	112663	214803	38.99%	4.916%
8	6.694	1649	1665	1687	rBV	124864	239210	43.43%	5.474%
9	7.568	1925	1937	1952	rBV	57771	100676	18.28%	2.304%
10	7.903	2026	2041	2059	rBV	216706	395948	71.88%	9.061%
11	8.182	2116	2128	2143	rBV	36973	62120	11.28%	1.422%
12	8.475	2208	2219	2231	rBV3	7399	13163	2.39%	0.301%
13	8.555	2231	2244	2258	rBV2	206117	358936	65.16%	8.214%
14	8.636	2258	2269	2315	rVB	298063	550849	100.00%	12.606%
15	9.420	2498	2513	2531	rBV	183705	316342	57.43%	7.240%
16	10.758	2916	2929	2944	rVB	99297	159733	29.00%	3.656%
17	10.893	2962	2971	2982	rBV2	6400	9761	1.77%	0.223%
18	11.812	3245	3257	3274	rBV	179129	283077	51.39%	6.478%
19	12.195	3362	3376	3389	rBV	213443	343771	62.41%	7.867%




Sum of corrected areas: 4369600

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020422\
Data File : VU047054.D
Acq On : 04 Feb 2022 18:46
Operator : SY/MD
Sample : VIBLK037
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK037

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

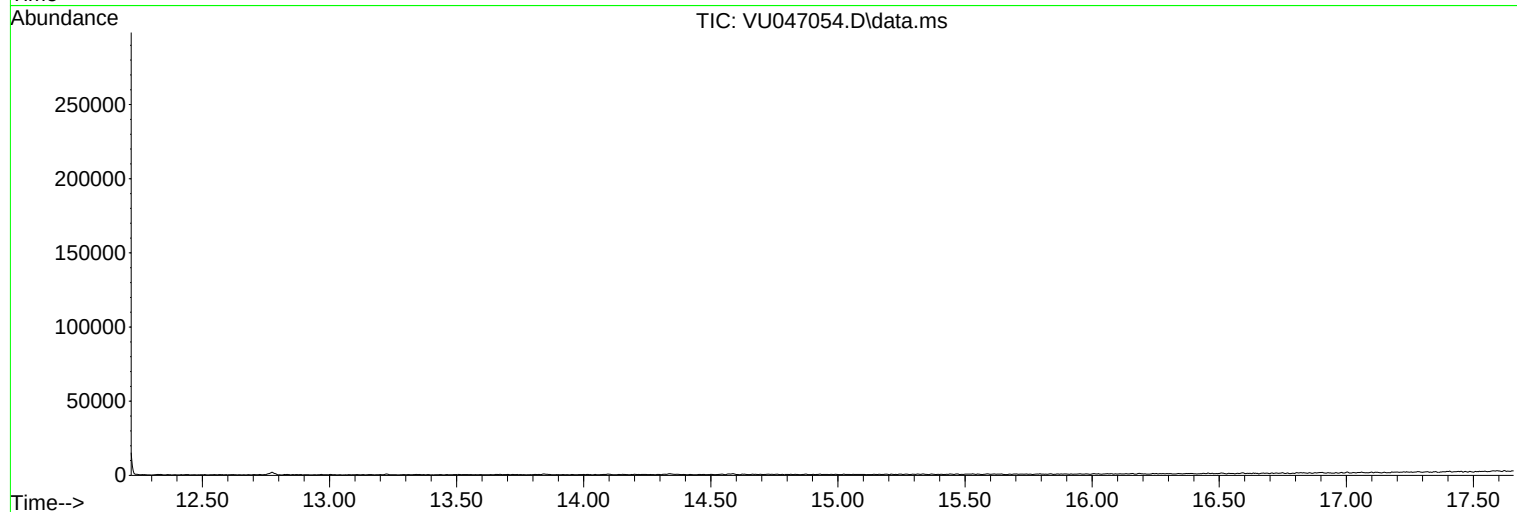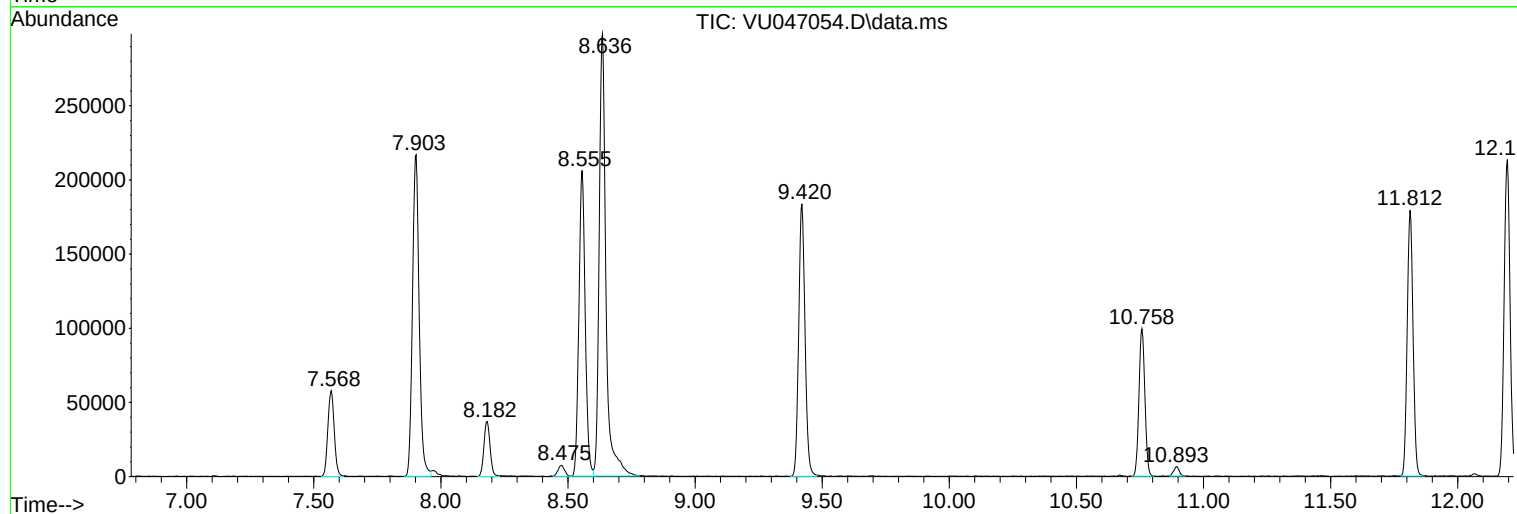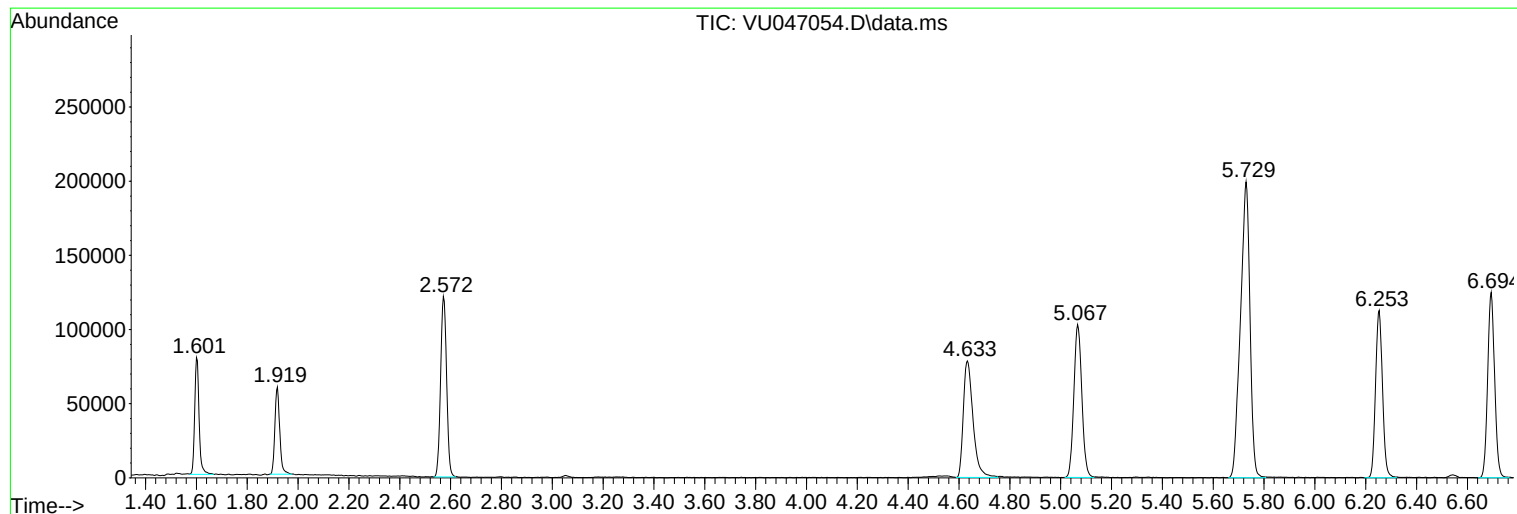

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020422\
Data File : VU047054.D
Acq On : 04 Feb 2022 18:46
Operator : SY/MD
Sample : VIBLK037
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK037

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020422\
Data File : VU047054.D
Acq On : 04 Feb 2022 18:46
Operator : SY/MD
Sample : VIBLK037
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK037

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc