
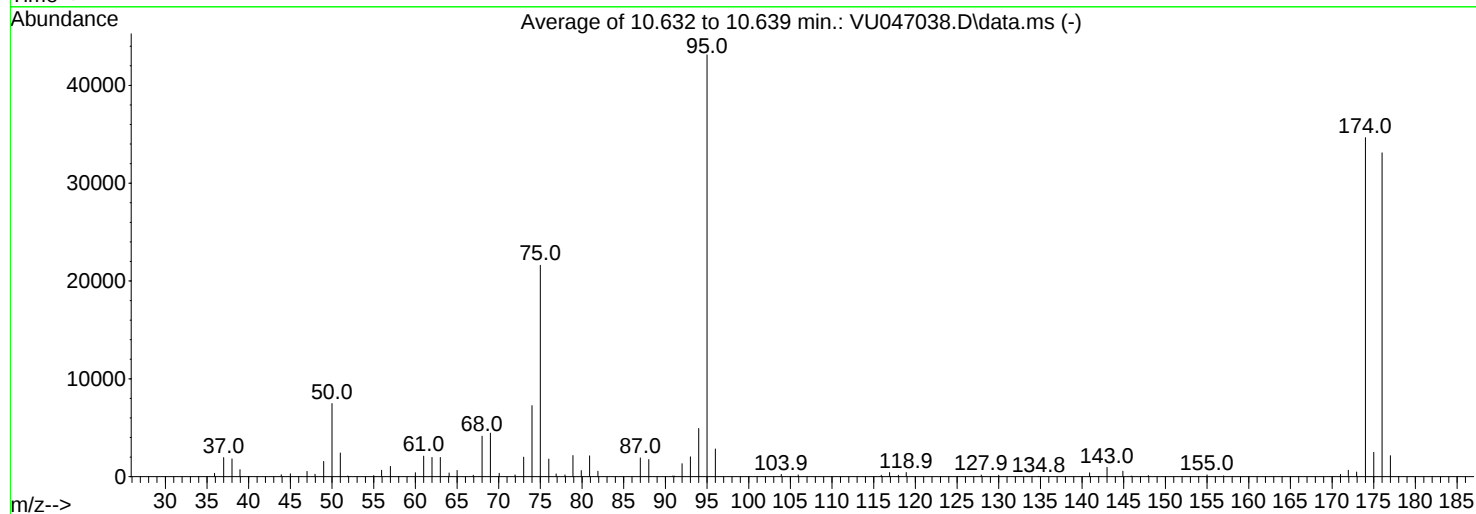


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020422\
 Data File : VU047038.D
 Acq On : 04 Feb 2022 09:26
 Operator : SY/MD
 Sample : BFB054
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB054

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020422WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Feb 05 01:18:17 2022

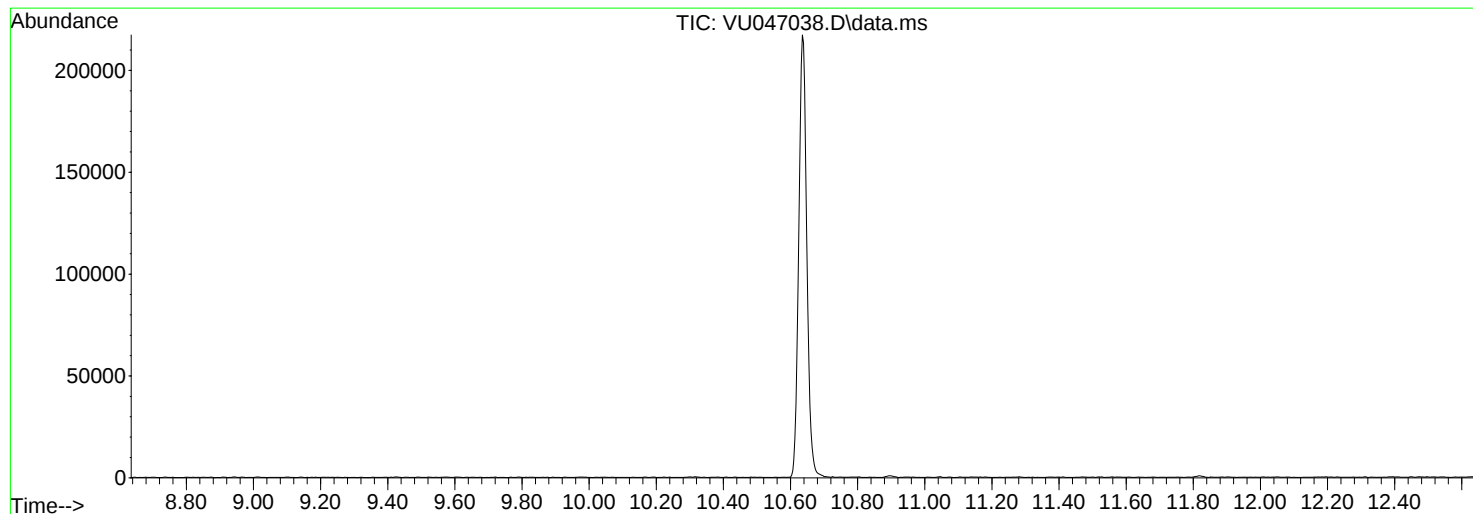

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	7475	PASS
75	95	30	80	50.1	21613	PASS
95	95	100	100	100.0	43123	PASS
96	95	5	9	6.6	2835	PASS
173	174	0.00	2	1.4	478	PASS
174	95	50	120	80.4	34659	PASS
175	174	5	9	7.2	2482	PASS
176	174	95	101	95.5	33112	PASS
177	176	5	9	6.5	2148	PASS

m/z	Abundance
39.90	111.0
43.90	207.0

Instrument :
MSVOA_U
ClientSampleId :
BFB054

m/z	Abundance
35.90	332.0
37.00	1950.0
38.00	1796.0
39.00	658.0
40.10	134.0
43.90	418.0
45.00	289.0
47.00	528.0
47.90	214.0
49.00	1592.0
50.00	7228.0
51.00	2373.0
55.00	113.0
55.90	658.0
57.00	976.0
60.00	416.0
61.00	2139.0
62.00	1968.0
63.00	1891.0
64.10	336.0
65.00	647.0
67.00	143.0
68.00	3834.0
69.00	4251.0
70.10	388.0
72.00	132.0
73.00	1982.0
74.00	6876.0
75.00	20688.0
76.00	1766.0
76.90	288.0
77.90	174.0
78.90	2084.0
79.90	581.0
80.90	2148.0
81.90	520.0
87.00	1881.0
88.00	1851.0
90.90	113.0
92.00	1264.0
93.00	1966.0
94.00	4789.0
95.00	42024.0
96.00	2690.0
103.90	251.0
106.00	163.0
115.90	182.0
116.90	435.0
117.90	168.0
118.90	415.0
127.90	132.0
130.00	148.0
140.90	393.0
143.00	864.0
144.90	529.0
147.90	113.0
155.00	142.0
171.00	220.0
171.90	560.0
172.90	426.0
174.00	32640.0
175.00	2290.0
176.00	31224.0
177.00	2147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB054

m/z	Abundance
35.90	371.0
37.00	2014.0
38.00	1920.0
39.00	728.0
40.00	120.0
43.90	389.0
45.00	315.0
47.00	557.0
48.00	258.0
49.00	1585.0
50.00	7734.0
51.00	2475.0
51.90	101.0
55.00	129.0
56.00	661.0
57.00	1106.0
60.00	423.0
61.00	2136.0
62.00	1968.0
63.00	2026.0
64.00	386.0
65.00	662.0
66.90	170.0
68.00	4287.0
69.00	4611.0
70.00	373.0
71.90	178.0
73.00	2071.0
74.00	7438.0
75.00	22168.0
76.00	1855.0
76.90	301.0
77.90	187.0
78.90	2263.0
79.90	653.0
80.90	2193.0
81.90	582.0
87.00	1976.0
88.00	1780.0
90.90	124.0
92.00	1340.0
93.00	2075.0
94.00	5068.0
95.00	44360.0
96.00	2912.0
103.90	226.0
105.90	180.0
115.90	142.0
116.90	439.0
118.00	152.0
118.90	439.0
127.90	151.0
130.00	143.0
134.80	100.0
140.90	412.0
143.00	987.0
144.90	592.0
145.90	112.0
147.90	111.0
155.00	191.0
157.00	129.0
171.00	236.0
171.90	680.0
173.00	496.0
174.00	35560.0
175.00	2564.0
176.00	34032.0
177.00	2220.0

Instrument :
MSVOA_U
ClientSampleId :
BFB054

m/z	Abundance
35.90	318.0
37.00	1855.0
38.00	1753.0
38.90	780.0
39.90	105.0
43.90	383.0
45.00	299.0
47.00	531.0
48.00	268.0
49.00	1496.0
50.00	7462.0
51.00	2397.0
51.90	112.0
55.00	114.0
56.00	625.0
57.00	1052.0
60.00	384.0
61.00	2035.0
62.00	1960.0
63.00	1955.0
64.00	407.0
65.00	621.0
66.90	151.0
68.00	4318.0
69.00	4501.0
70.00	269.0
71.90	224.0
73.00	1952.0
74.00	7460.0
75.00	21984.0
76.00	1764.0
76.90	265.0
78.00	179.0
78.90	2141.0
79.90	633.0
80.90	2044.0
81.90	578.0
87.00	1891.0
88.00	1614.0
91.10	126.0
92.00	1369.0
93.00	2069.0
94.00	4943.0
95.00	42984.0
96.00	2902.0
103.90	195.0
105.90	181.0
115.90	125.0
116.90	394.0
118.00	122.0
118.90	423.0
127.90	184.0
130.00	145.0
140.90	385.0
143.00	996.0
144.90	555.0
145.90	112.0
148.00	100.0
155.00	204.0
157.00	105.0
171.00	248.0
172.00	724.0
173.00	511.0
174.00	35776.0
175.00	2593.0
176.00	34080.0
177.00	2076.0

Instrument :
MSVOA_U
ClientSampleId :
BFB054