

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020425\
 Data File : VU063126.D
 Acq On : 04 Feb 2025 18:05
 Operator : MD/SY
 Sample : Q1227-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E2973

Quant Time: Feb 05 08:04:03 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020425WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 05 07:57:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.239	114	86538	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	83212	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	33412	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	23233	4.694	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	93.800%	
7) Chloroethane-d5	1.901	69	21587	4.699	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	94.000%	
11) 1,1-Dichloroethene-d2	2.554	65	10603	4.798	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	96.000%	
20) 2-Butanone-d5	4.608	46	73798	45.288	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	90.580%	
24) Chloroform-d	5.049	84	48916	4.470	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	89.400%	
26) 1,2-Dichloroethane-d4	5.689	65	26581	4.722	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.400%	
32) Benzene-d6	5.714	84	98224	4.525	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.600%	
36) 1,2-Dichloropropane-d6	6.679	67	33036	4.617	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	92.400%	
41) Toluene-d8	7.888	98	82002	4.277	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.600%	
43) trans-1,3-Dichloroprop...	8.171	79	11447	4.269	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	85.400%	
46) 2-Hexanone-d5	8.621	63	55914	41.434	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	82.860%	
56) 1,1,2,2-Tetrachloroeth...	10.746	84	27437	4.344	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	86.800%	
66) 1,2-Dichlorobenzene-d4	12.184	152	27559	4.940	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	98.800%	
Target Compounds					Qvalue	
13) Acetone	2.615	43	15480	15.085	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020425\
Data File : VU063126.D
Acq On : 04 Feb 2025 18:05
Operator : MD/SY
Sample : Q1227-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2973

Quant Time: Feb 05 08:04:03 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 05 07:57:12 2025
Response via : Initial Calibration

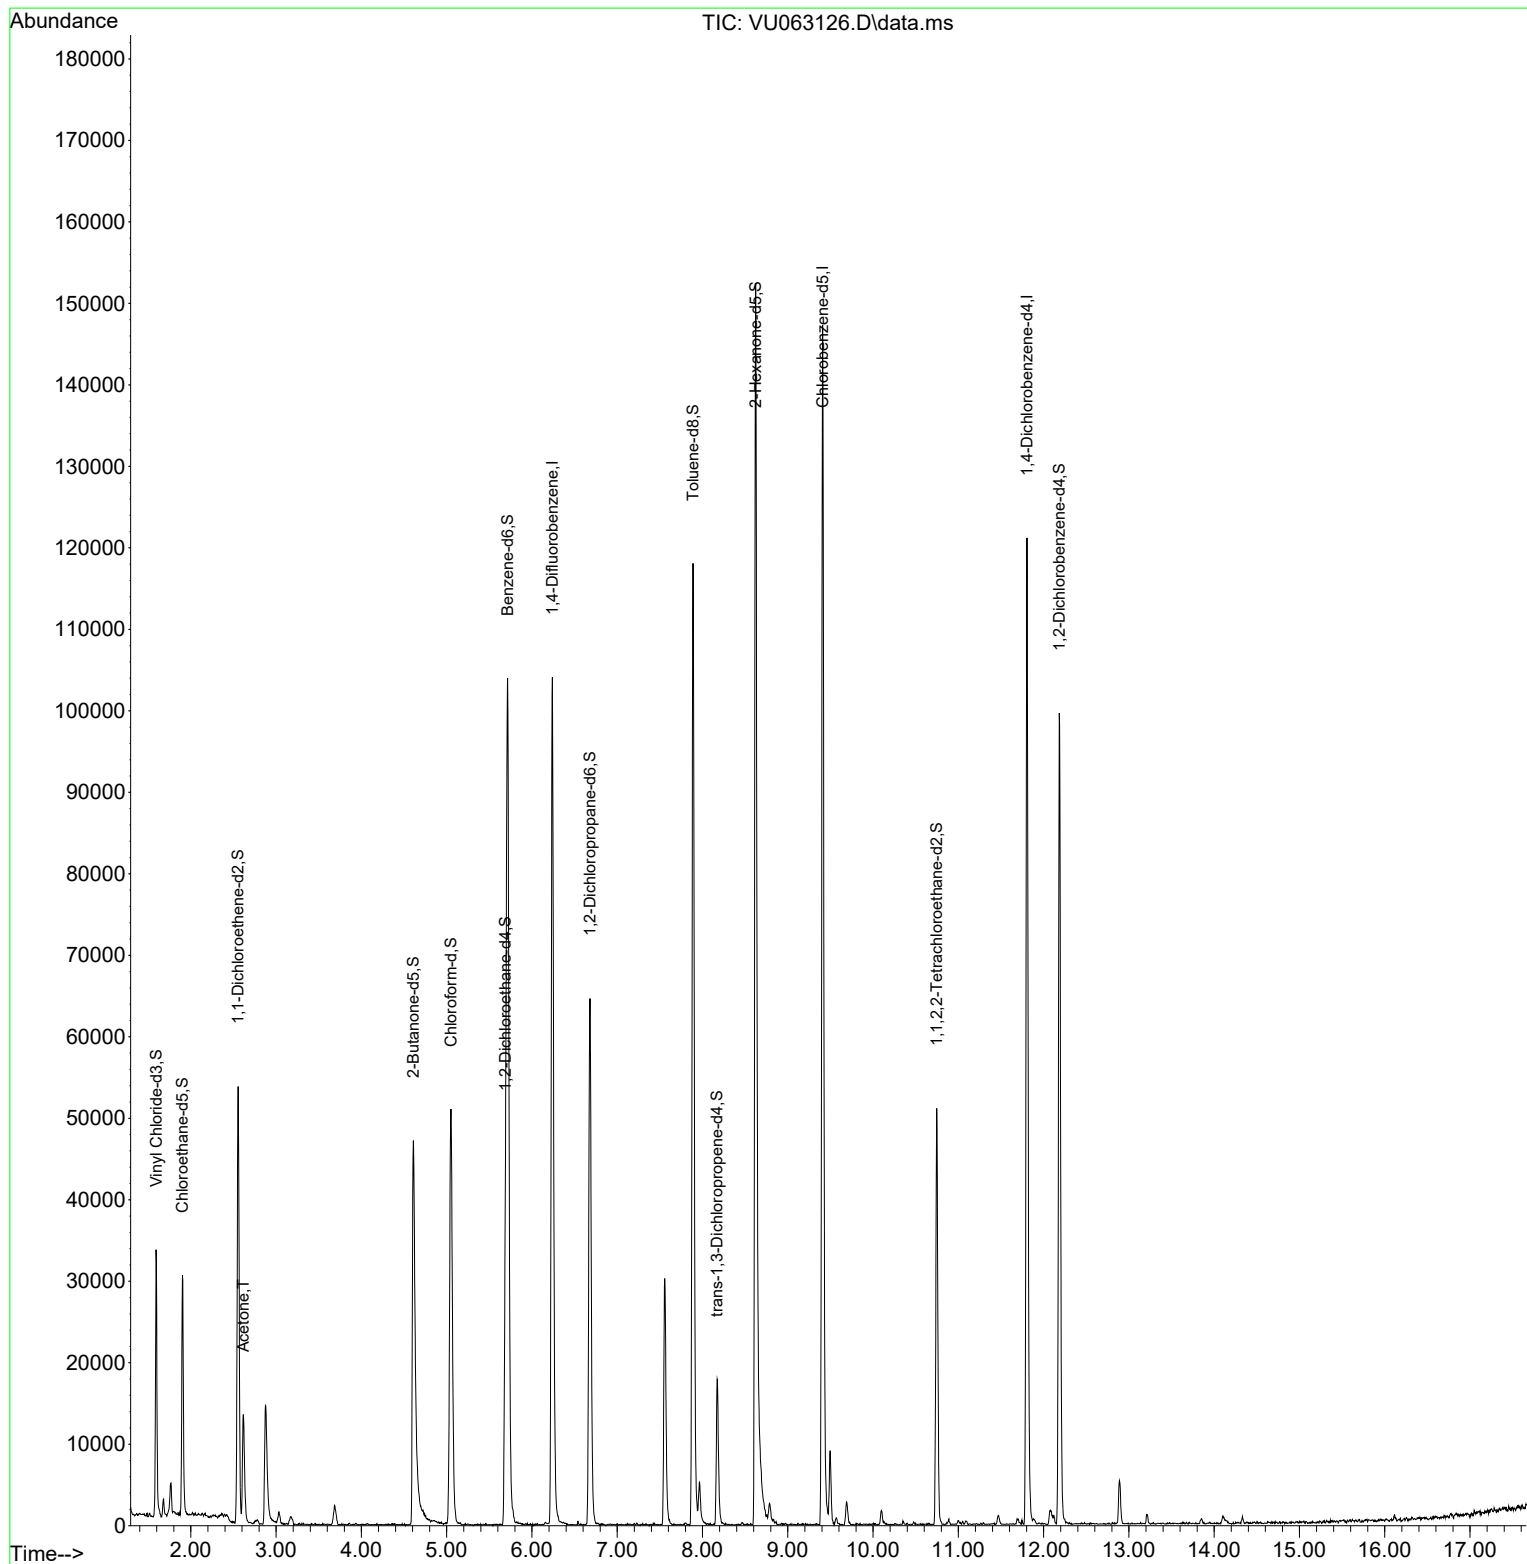

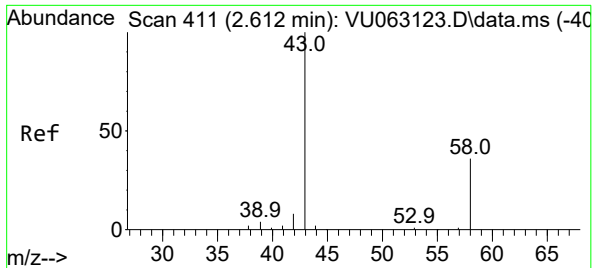

#13
 Acetone
 Concen: 15.085 ug/L
 RT: 2.615 min Scan# 41
 Delta R.T. 0.003 min
 Lab File: VU063126.D
 Acq: 04 Feb 2025 18:05

Instrument :
 MSVOA_U
 ClientSampleId :
 E2973

Tgt Ion: 43 Resp: 15480
 Ion Ratio Lower Upper
 43 100
 58 32.5 0.0 70.2

