

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020425\
 Data File : VU063137.D
 Acq On : 04 Feb 2025 22:40
 Operator : MD/SY
 Sample : Q1227-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E2987

Quant Time: Feb 05 08:06:36 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020425WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 05 07:57:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.239	114	78250	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	75619	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	31893	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	20832	4.654	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	93.000%	
7) Chloroethane-d5	1.901	69	19218	4.626	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	92.600%	
11) 1,1-Dichloroethene-d2	2.554	65	9379	4.694	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	93.800%	
20) 2-Butanone-d5	4.608	46	69919	47.452	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	94.900%	
24) Chloroform-d	5.049	84	45068	4.554	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.000%	
26) 1,2-Dichloroethane-d4	5.689	65	23878	4.691	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	93.800%	
32) Benzene-d6	5.714	84	89171	4.521	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.400%	
36) 1,2-Dichloropropane-d6	6.679	67	29627	4.556	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	91.200%	
41) Toluene-d8	7.888	98	73956	4.244	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	84.800%	
43) trans-1,3-Dichloroprop...	8.171	79	9871	4.051	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	81.000%	
46) 2-Hexanone-d5	8.621	63	52121	42.502	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	85.000%	
56) 1,1,2,2-Tetrachloroeth...	10.746	84	25216	4.393	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	87.800%	
66) 1,2-Dichlorobenzene-d4	12.184	152	25261	4.743	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	94.800%	
Target Compounds						Qvalue
13) Acetone	2.615	43	13085	14.102	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020425\
Data File : VU063137.D
Acq On : 04 Feb 2025 22:40
Operator : MD/SY
Sample : Q1227-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2987

Quant Time: Feb 05 08:06:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 05 07:57:12 2025
Response via : Initial Calibration

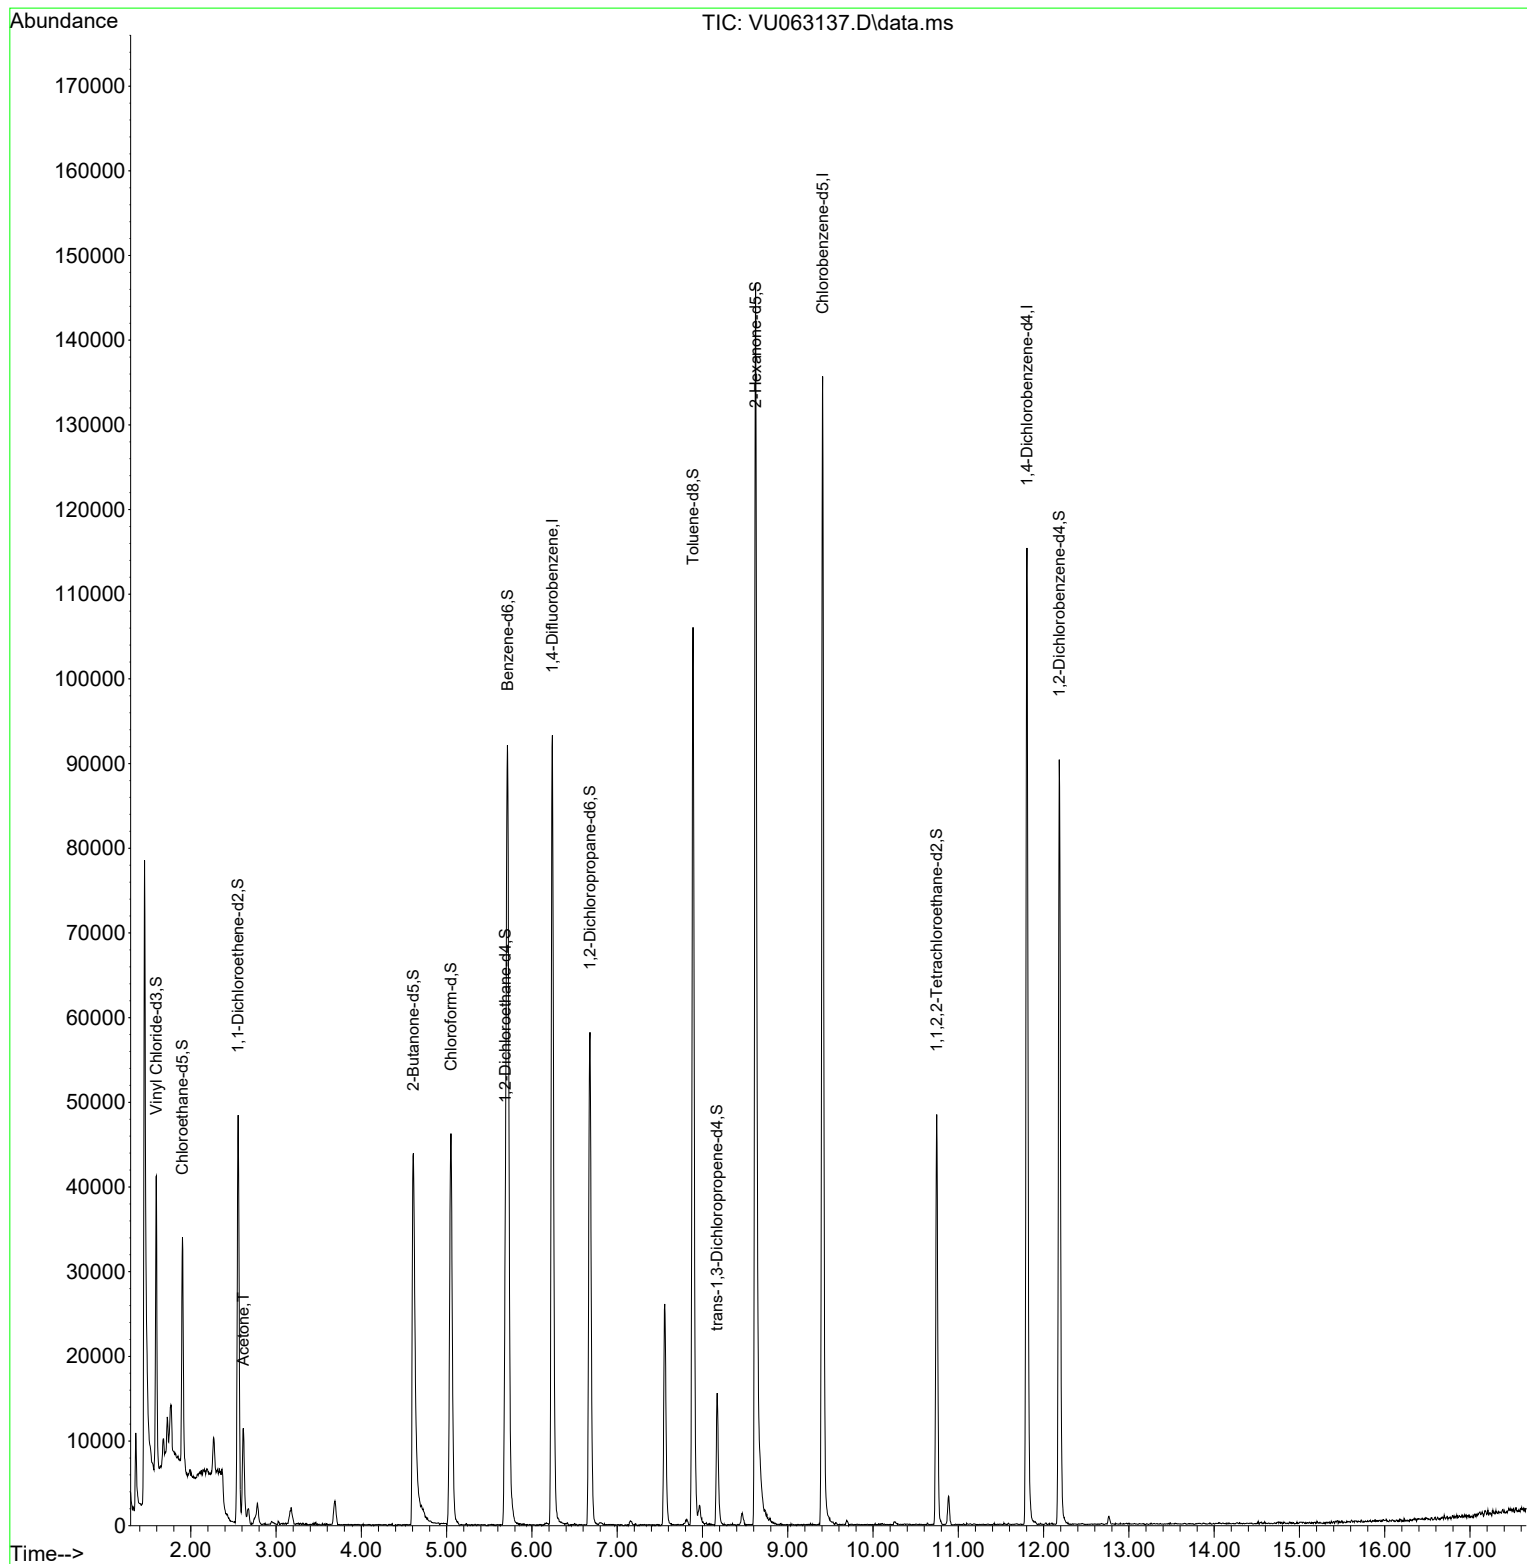

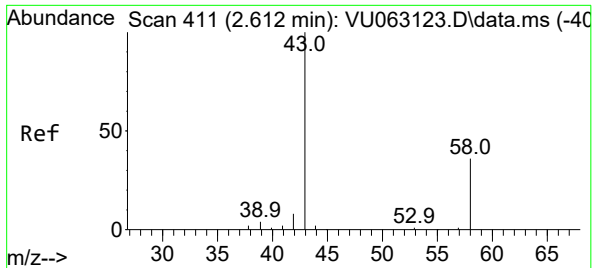

#13
 Acetone
 Concen: 14.102 ug/L
 RT: 2.615 min Scan# 41
 Delta R.T. 0.003 min
 Lab File: VU063137.D
 Acq: 04 Feb 2025 22:40

Instrument :
 MSVOA_U
 ClientSampleId :
 E2987

Tgt Ion: 43 Resp: 13085
 Ion Ratio Lower Upper
 43 100
 58 34.4 0.0 70.2

