


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020425\
Data File : VU063115.D
Acq On : 04 Feb 2025 11:44
Operator : MD/SY
Sample : BFB072
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB072

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020425WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Feb 06 07:25:52 2025

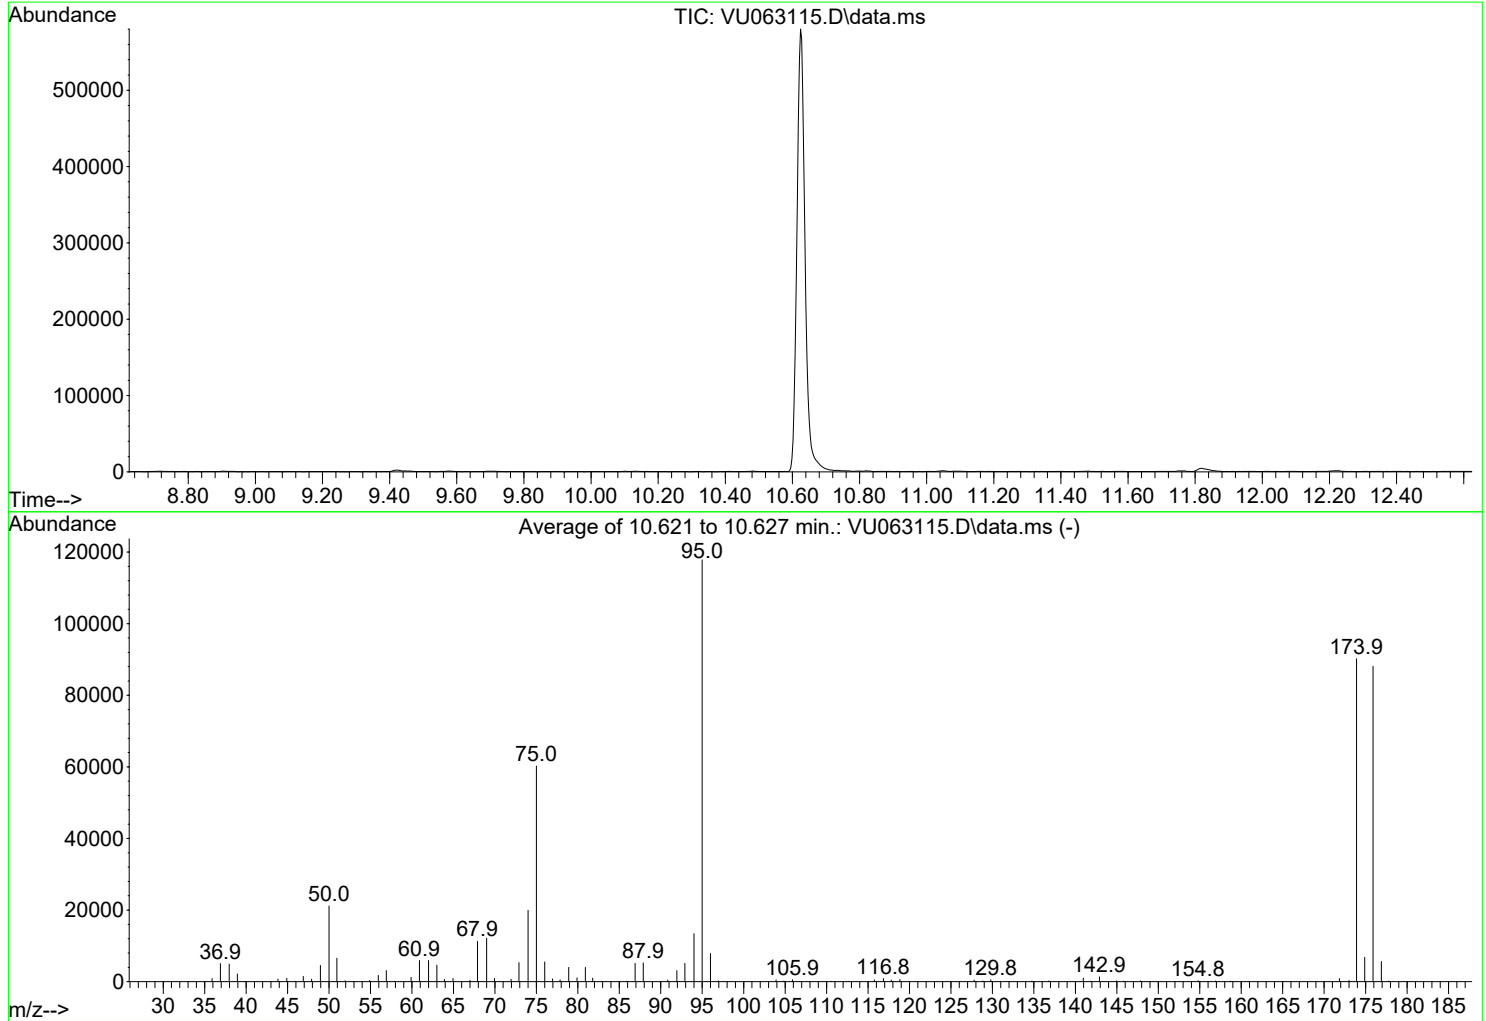

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.9	21149	PASS
75	95	30	80	51.1	60267	PASS
95	95	100	100	100.0	117829	PASS
96	95	5	9	6.7	7855	PASS
173	174	0.00	2	0.4	318	PASS
174	95	50	120	76.6	90213	PASS
175	174	5	9	7.5	6792	PASS
176	174	95	101	97.6	88091	PASS
177	176	5	9	6.4	5640	PASS

m/z	Abundance
39.80	190.0
43.70	289.0

Instrument :
MSVOA_U
ClientSampleId :
BFB072

m/z	Abundance
35.90	868.0
36.90	4969.0
38.00	4775.0
38.90	2028.0
39.90	216.0
43.90	968.0
44.90	879.0
45.90	111.0
46.90	1533.0
47.90	634.0
48.90	4354.0
50.00	20448.0
50.90	6260.0
51.90	297.0
52.90	106.0
54.90	331.0
55.90	1758.0
56.90	3132.0
57.90	112.0
59.90	1244.0
60.90	5747.0
62.00	5856.0
63.00	4487.0
63.90	668.0
64.90	882.0
66.00	116.0
67.00	372.0
67.90	10624.0
69.00	12026.0
69.90	989.0
71.90	613.0
72.90	5123.0
74.00	19312.0
75.00	58616.0
76.00	5258.0
77.00	676.0
77.90	508.0
78.90	3896.0
79.90	1027.0
80.90	3838.0
81.80	975.0
82.90	114.0
85.80	109.0
86.90	4980.0
87.90	5013.0
90.80	497.0
92.00	2929.0
92.90	4915.0
94.00	12831.0
95.00	113624.0
96.00	7764.0
96.90	200.0
103.90	475.0
104.80	177.0
105.90	512.0
110.60	109.0
115.70	466.0
116.80	802.0
117.80	407.0
118.90	546.0
127.80	482.0
128.80	182.0
129.80	495.0
131.00	133.0
134.70	173.0
136.80	200.0
140.90	950.0
141.80	115.0
142.90	1206.0
144.90	204.0
145.80	153.0
147.90	199.0
154.80	293.0
156.90	178.0
158.70	147.0
171.90	821.0
173.90	86040.0
174.90	6430.0
175.90	82688.0
176.90	5166.0
177.80	166.0

Instrument :
MSVOA_U
ClientSampleId :
BFB072

m/z	Abundance
35.90	885.0
36.90	5229.0
38.00	5096.0
39.00	2244.0
39.80	225.0
43.90	1051.0
44.90	931.0
45.90	158.0
46.90	1570.0
47.90	677.0
49.00	4682.0
50.00	21760.0
50.90	6813.0
51.90	292.0
54.90	365.0
55.90	1841.0
56.90	3157.0
58.00	124.0
59.90	1255.0
60.90	6037.0
62.00	6069.0
63.00	4754.0
63.90	636.0
65.00	945.0
66.00	116.0
67.00	361.0
67.90	11573.0
69.00	12510.0
69.90	883.0
71.90	672.0
72.90	5491.0
74.00	20568.0
75.00	62272.0
76.00	5719.0
76.90	822.0
77.90	514.0
78.90	4127.0
79.90	1100.0
80.90	4157.0
81.80	997.0
82.90	116.0
85.90	138.0
86.90	5247.0
87.90	5438.0
90.80	454.0
92.00	3241.0
92.90	5296.0
94.00	13765.0
95.00	121424.0
96.00	8168.0
96.90	219.0
103.90	532.0
104.90	182.0
105.90	584.0
110.60	121.0
112.70	109.0
115.70	529.0
116.80	894.0
117.80	483.0
118.90	654.0
127.80	472.0
128.80	161.0
129.80	564.0
131.00	143.0
134.80	191.0
136.80	217.0
140.90	1011.0
141.90	140.0
142.90	1366.0
144.90	262.0
145.80	160.0
147.80	213.0
154.80	276.0
156.90	192.0
158.70	167.0
160.90	144.0
171.90	886.0
173.90	93056.0
174.90	7045.0
175.90	91288.0
176.90	5823.0
177.80	205.0

Instrument :
MSVOA_U
ClientSampleId :
BFB072

m/z	Abundance
35.90	814.0
36.90	4980.0
37.90	4881.0
39.00	2168.0
39.80	213.0
43.90	1026.0
44.90	959.0
45.90	170.0
46.90	1391.0
47.90	703.0
49.00	4498.0
50.00	21240.0
51.00	6659.0
52.00	280.0
54.90	382.0
56.00	1663.0
56.90	3020.0
58.00	117.0
59.90	1135.0
60.90	5871.0
62.00	5819.0
63.00	4512.0
63.90	587.0
65.00	874.0
65.90	102.0
67.00	292.0
67.90	11647.0
69.00	11786.0
70.00	798.0
72.00	704.0
72.90	5362.0
74.00	19992.0
75.00	59912.0
76.00	5530.0
76.90	829.0
77.80	519.0
78.90	3979.0
79.90	1085.0
80.90	3974.0
81.80	945.0
82.80	108.0
86.00	137.0
86.90	5057.0
87.90	5213.0
90.90	406.0
91.90	3110.0
92.90	5090.0
94.00	13591.0
95.00	118440.0
96.00	7634.0
97.00	201.0
103.90	539.0
104.90	190.0
105.90	568.0
106.80	118.0
112.70	110.0
115.80	477.0
116.90	821.0
117.80	502.0
118.80	720.0
127.80	413.0
128.90	139.0
129.80	513.0
130.90	131.0
134.80	204.0
136.80	224.0
141.00	954.0
141.90	161.0
142.90	1444.0
145.00	263.0
145.80	151.0
147.80	203.0
154.80	230.0
156.90	183.0
158.70	138.0
160.90	171.0
171.80	892.0
173.00	954.0
173.90	91544.0
174.90	6902.0
175.90	90296.0
176.90	5931.0
177.80	173.0

Instrument :
MSVOA_U
ClientSampleId :
BFB072