

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020525\
 Data File : VU063179.D
 Acq On : 06 Feb 2025 00:32
 Operator : MD/SY
 Sample : Q1226-25
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCZN7

Quant Time: Feb 06 08:11:31 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020425WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Feb 06 07:25:52 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	96699	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.405	117	91323	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	38725	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	22631	4.092	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.800%
7) Chloroethane-d5	1.904	69	23573	4.592	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.800%
11) 1,1-Dichloroethene-d2	2.557	65	10897	4.413	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	88.200%
20) 2-Butanone-d5	4.605	46	81556	44.789	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.580%
24) Chloroform-d	5.049	84	55040	4.501	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.000%
26) 1,2-Dichloroethane-d4	5.688	65	28767	4.574	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.400%
32) Benzene-d6	5.714	84	109221	4.585	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.800%
36) 1,2-Dichloropropane-d6	6.679	67	36659	4.668	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.400%
41) Toluene-d8	7.888	98	90467	4.299	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.000%
43) trans-1,3-Dichloroprop...	8.171	79	11956	4.063	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.200%
46) 2-Hexanone-d5	8.621	63	62649	42.302	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.600%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	29977	4.325	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.400%
66) 1,2-Dichlorobenzene-d4	12.183	152	31229	4.829	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.600%
Target Compounds						Qvalue
13) Acetone	2.618	43	5296	4.619	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020525\
Data File : VU063179.D
Acq On : 06 Feb 2025 00:32
Operator : MD/SY
Sample : Q1226-25
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCZN7


Quant Time: Feb 06 08:11:31 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Feb 06 07:25:52 2025
Response via : Initial Calibration

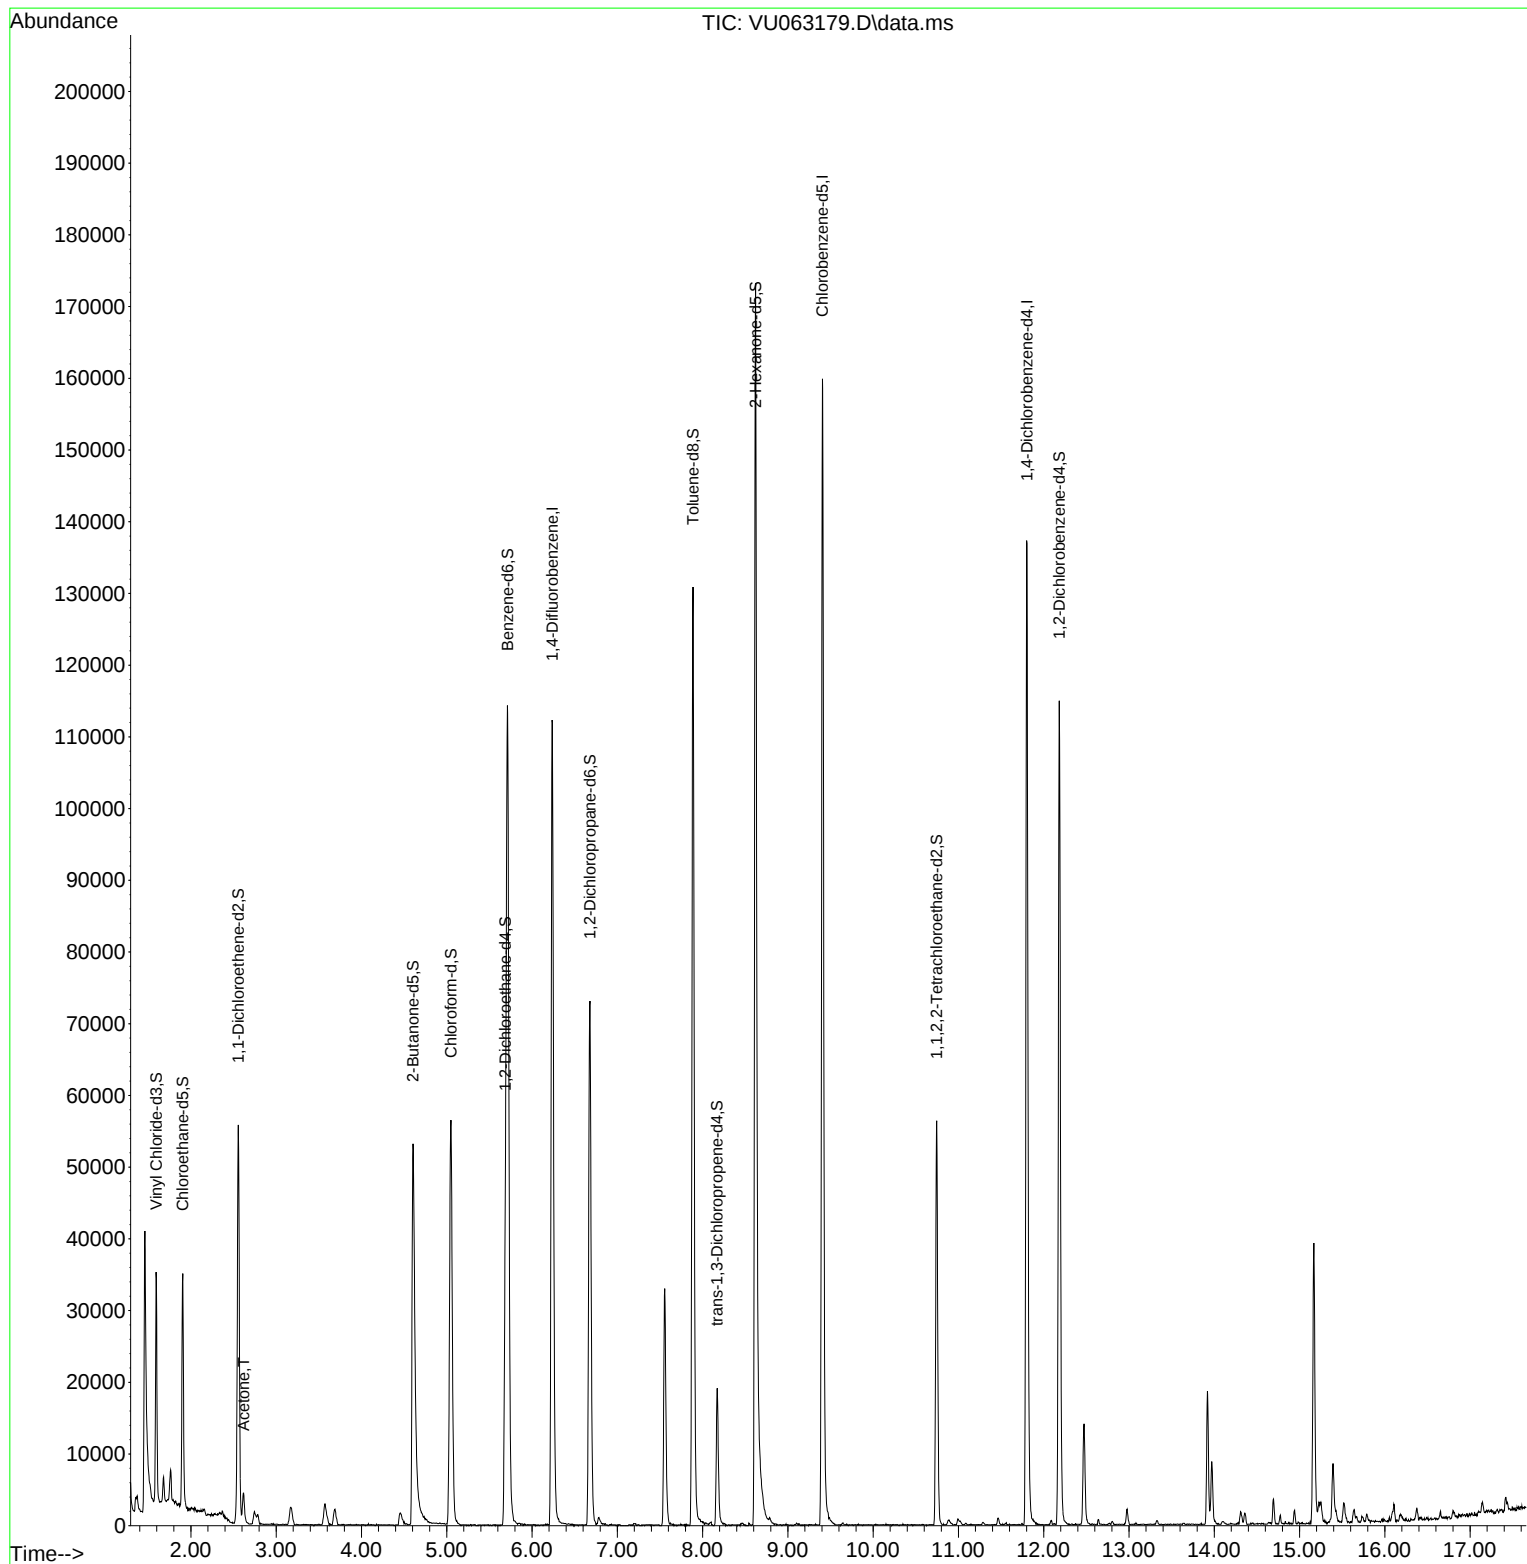

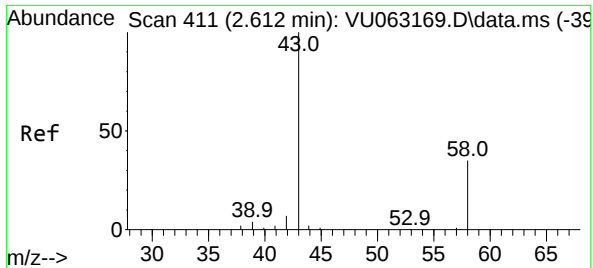

#13
Acetone
Concen: 4.619 ug/L
RT: 2.618 min Scan# 41
Delta R.T. 0.006 min
Lab File: VU063179.D
Acq: 06 Feb 2025 00:32

Instrument :
MSVOA_U
ClientSampleId :
DCZN7

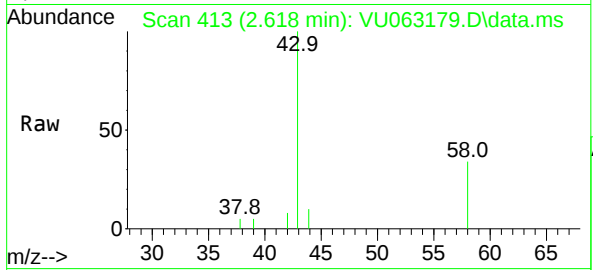

Tgt Ion: 43 Resp: 5296
Ion Ratio Lower Upper
43 100
58 30.9 0.0 70.2

