


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020525\
Data File : VU063145.D
Acq On : 05 Feb 2025 08:13
Operator : MD/SY
Sample : BFB073
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB073

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020425WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Feb 07 07:28:28 2025

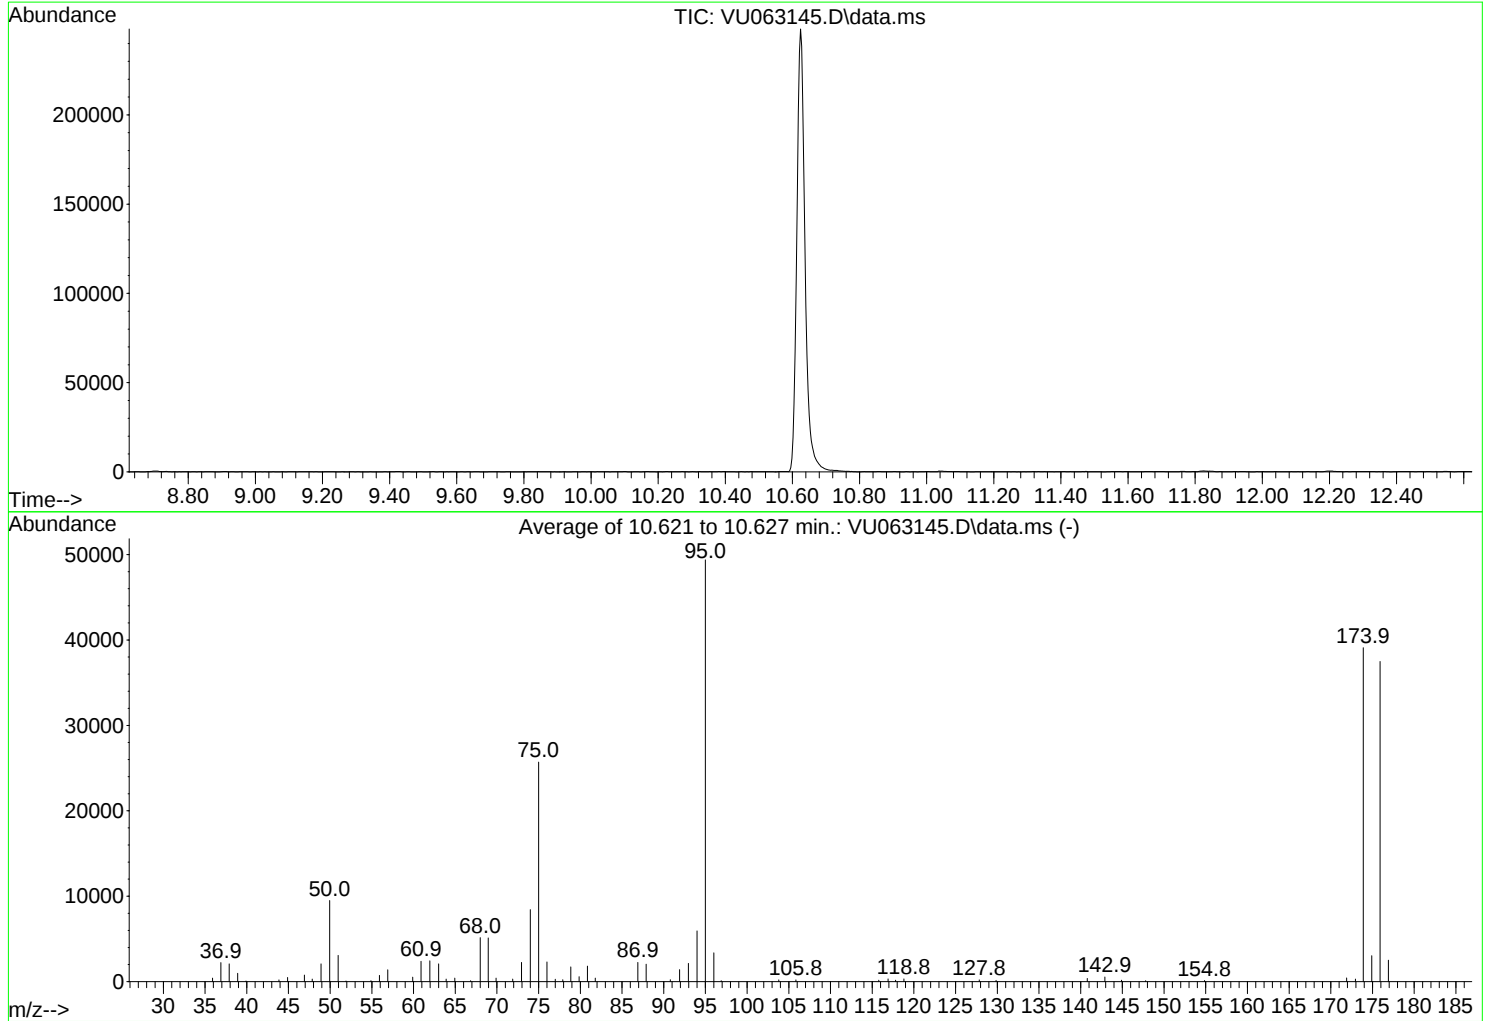

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	9495	PASS
75	95	30	80	52.0	25704	PASS
95	95	100	100	100.0	49384	PASS
96	95	5	9	6.8	3372	PASS
173	174	0.00	2	0.8	298	PASS
174	95	50	120	79.2	39093	PASS
175	174	5	9	7.7	3029	PASS
176	174	95	101	95.9	37477	PASS
177	176	5	9	6.7	2504	PASS

m/z	Abundance
43.90	161.0

Instrument :
MSVOA_U
ClientSampleId :
BFB073

m/z	Abundance
35.90	416.0
36.90	2189.0
37.90	2105.0
38.90	1002.0
39.90	110.0
43.90	350.0
44.90	501.0
46.90	735.0
47.80	303.0
48.90	2097.0
50.00	9436.0
51.00	3026.0
51.90	110.0
54.90	117.0
55.90	706.0
56.90	1391.0
59.90	577.0
60.90	2420.0
61.90	2390.0
63.00	2048.0
63.90	317.0
64.90	407.0
66.90	118.0
68.00	5076.0
68.90	5175.0
69.90	395.0
71.90	310.0
72.90	2152.0
74.00	8396.0
75.00	25280.0
76.00	2266.0
77.00	302.0
77.90	223.0
78.90	1745.0
79.90	578.0
80.80	1788.0
81.80	442.0
86.90	2314.0
87.90	2079.0
90.80	194.0
91.90	1417.0
93.00	2036.0
94.00	5839.0
95.00	48312.0
96.00	3411.0
96.90	109.0
103.80	176.0
105.90	239.0
115.80	156.0
116.90	328.0
117.80	177.0
118.80	329.0
127.90	194.0
129.90	139.0
140.80	406.0
142.90	543.0
144.90	151.0
147.80	103.0
154.90	129.0
171.90	368.0
173.90	37672.0
174.90	2923.0
175.90	35632.0
176.90	2424.0

Instrument :
MSVOA_U
ClientSampleId :
BFB073

m/z	Abundance
35.90	433.0
36.90	2285.0
37.90	2175.0
38.90	1013.0
39.90	111.0
43.80	383.0
44.90	518.0
46.90	804.0
47.90	302.0
48.90	2140.0
49.90	9777.0
50.90	3183.0
51.90	110.0
54.90	121.0
55.90	758.0
56.90	1448.0
59.90	551.0
60.90	2473.0
61.90	2536.0
63.00	2138.0
63.90	319.0
64.90	438.0
66.80	121.0
68.00	5367.0
69.00	5257.0
69.90	425.0
71.90	312.0
72.90	2320.0
74.00	8664.0
75.00	26560.0
76.00	2371.0
77.00	294.0
77.90	222.0
78.90	1809.0
79.90	622.0
80.90	1863.0
81.80	426.0
86.90	2328.0
87.90	2072.0
90.80	228.0
91.90	1436.0
93.00	2224.0
94.00	6132.0
95.00	50808.0
96.00	3480.0
96.90	117.0
103.80	211.0
105.80	212.0
115.80	173.0
116.90	311.0
117.80	184.0
118.80	318.0
127.90	209.0
129.80	148.0
140.80	383.0
142.90	581.0
144.90	186.0
147.80	118.0
154.80	151.0
171.90	448.0
173.00	464.0
173.90	40088.0
174.90	3139.0
175.90	38672.0
176.90	2609.0

Instrument :
MSVOA_U
ClientSampleId :
BFB073

m/z	Abundance
35.90	406.0
36.90	2235.0
37.90	1958.0
38.90	902.0
43.80	376.0
44.90	462.0
46.90	762.0
47.90	283.0
48.90	2015.0
49.90	9271.0
50.90	3011.0
54.90	119.0
55.90	724.0
56.90	1336.0
59.90	476.0
60.90	2262.0
62.00	2368.0
63.00	2076.0
63.90	255.0
65.00	425.0
66.80	121.0
68.00	5027.0
69.00	4896.0
69.90	391.0
71.90	281.0
73.00	2297.0
74.00	8208.0
75.00	25272.0
76.00	2268.0
77.00	246.0
77.90	232.0
78.80	1638.0
79.80	547.0
80.90	1788.0
81.80	365.0
86.90	2129.0
87.90	1968.0
90.80	235.0
91.90	1347.0
92.90	2172.0
94.00	5862.0
95.00	49032.0
96.00	3224.0
96.90	111.0
103.80	227.0
105.80	188.0
115.80	173.0
116.90	291.0
117.80	175.0
118.80	290.0
127.80	193.0
129.80	167.0
140.80	347.0
142.90	535.0
144.90	181.0
147.80	103.0
154.80	140.0
171.90	462.0
172.90	430.0
173.90	39520.0
174.90	3024.0
175.90	38128.0
176.90	2478.0

Instrument :
MSVOA_U
ClientSampleId :
BFB073