

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020625\
 Data File : VU063192.D
 Acq On : 06 Feb 2025 13:43
 Operator : MD/SY
 Sample : Q1226-09DL 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCZP1DL

Quant Time: Feb 07 07:29:53 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020425WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 07 07:28:28 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.235	114	85516	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	81085	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	32025	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	17933	3.666	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.400%
7) Chloroethane-d5	1.898	69	19176	4.224	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.400%
11) 1,1-Dichloroethene-d2	2.554	65	8774	4.018	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.400%
20) 2-Butanone-d5	4.605	46	70542	43.807	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.620%
24) Chloroform-d	5.049	84	47519	4.394	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.800%
26) 1,2-Dichloroethane-d4	5.689	65	25310	4.550	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.000%
32) Benzene-d6	5.714	84	90869	4.296	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.000%
36) 1,2-Dichloropropane-d6	6.676	67	31737	4.552	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.000%
41) Toluene-d8	7.888	98	74649	3.995	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.000%
43) trans-1,3-Dichloroprop...	8.171	79	10332	3.955	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.000%
46) 2-Hexanone-d5	8.621	63	49588	37.710	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.420%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	26344	4.280	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.600%
66) 1,2-Dichlorobenzene-d4	12.183	152	26009	4.864	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.200%
Target Compounds						
					Qvalue	
18) trans-1,2-Dichloroethene	3.341	96	1356	0.228	ug/L	89
22) cis-1,2-Dichloroethene	4.650	96	47468	7.159	ug/L	97
33) Benzene	5.766	78	3611	0.135	ug/L	100
34) Trichloroethene	6.531	95	16323	2.409	ug/L	97
47) Tetrachloroethene	8.544	164	5081	1.068	ug/L	98
51) Chlorobenzene	9.438	112	27689	1.645	ug/L	98
65) 1,4-Dichlorobenzene	11.827	146	3290	0.318	ug/L	99
67) 1,2-Dichlorobenzene	12.203	146	2902	0.301	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020625\
Data File : VU063192.D
Acq On : 06 Feb 2025 13:43
Operator : MD/SY
Sample : Q1226-09DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCZP1DL

Quant Time: Feb 07 07:29:53 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 07 07:28:28 2025
Response via : Initial Calibration




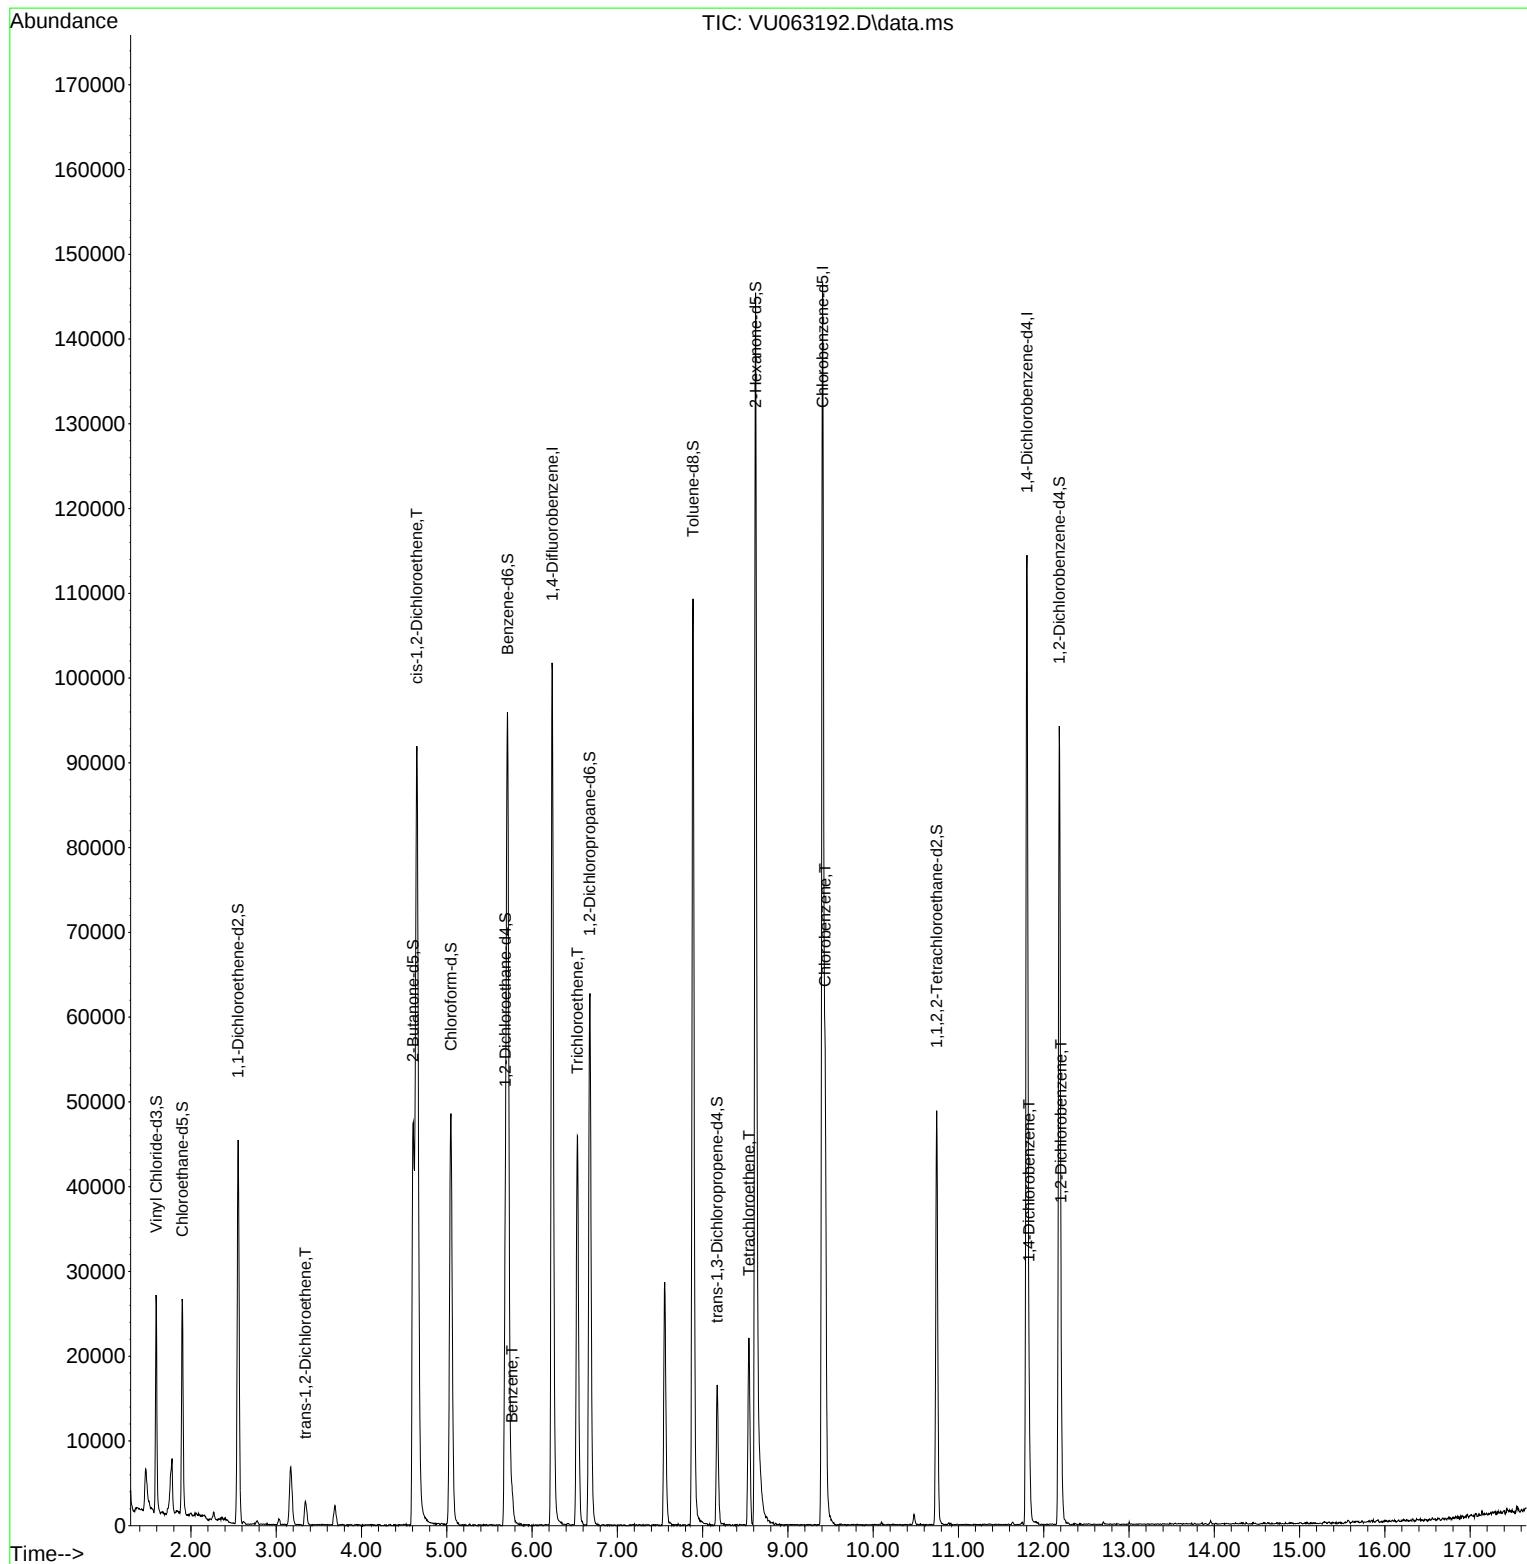


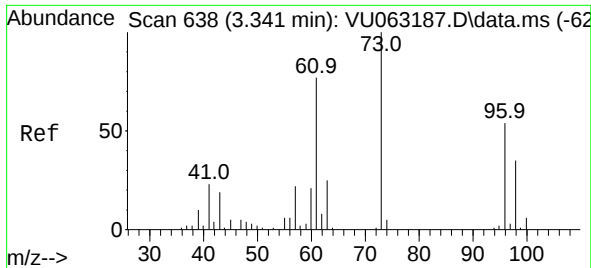

#18
trans-1,2-Dichloroethene
Concen: 0.228 ug/L
RT: 3.341 min Scan# 61
Delta R.T. -0.000 min
Lab File: VU063192.D
Acq: 06 Feb 2025 13:43




Instrument :
MSVOA_U
ClientSampleId :
DCZP1DL


Tgt Ion: 96 Resp: 1356
Ion Ratio Lower Upper
96 100
61 125.3 99.2 184.2
98 58.1 43.2 80.2

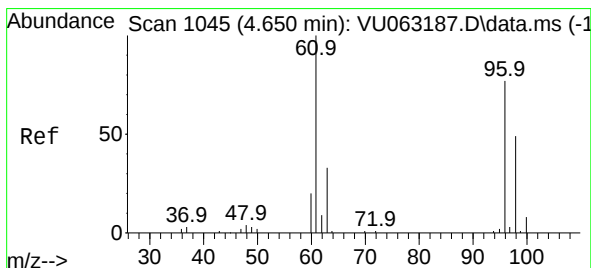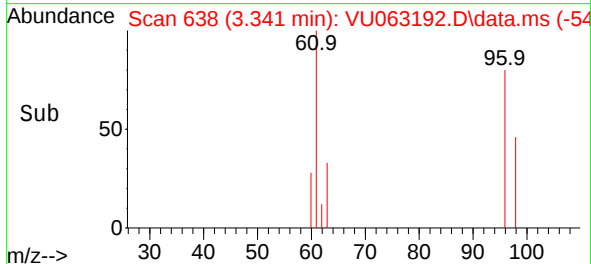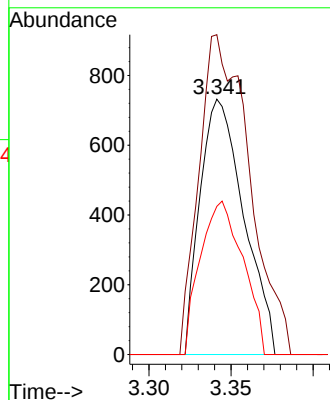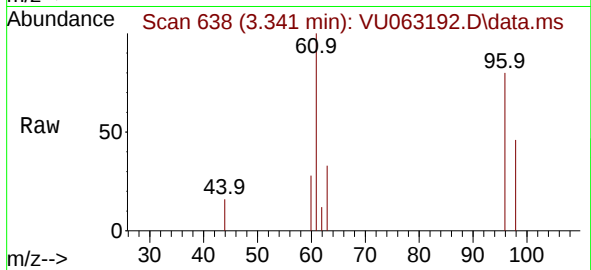

#22
cis-1,2-Dichloroethene
Concen: 7.159 ug/L
RT: 4.650 min Scan# 1045
Delta R.T. -0.000 min
Lab File: VU063192.D
Acq: 06 Feb 2025 13:43

Tgt Ion: 96 Resp: 47468
Ion Ratio Lower Upper
96 100
61 127.1 91.8 170.6
98 62.1 44.4 82.4

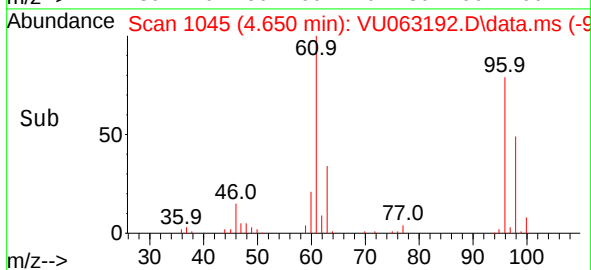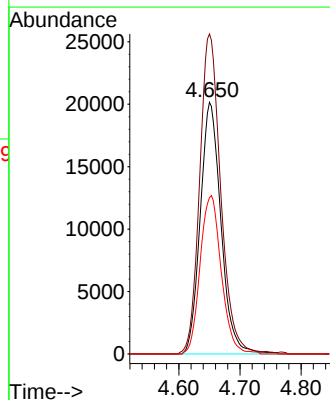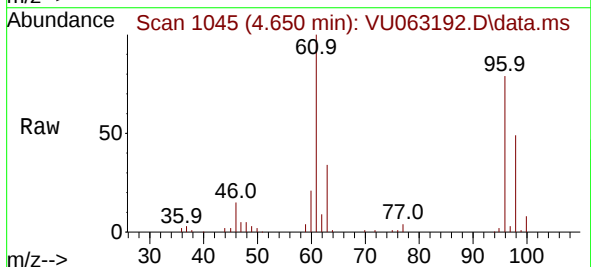

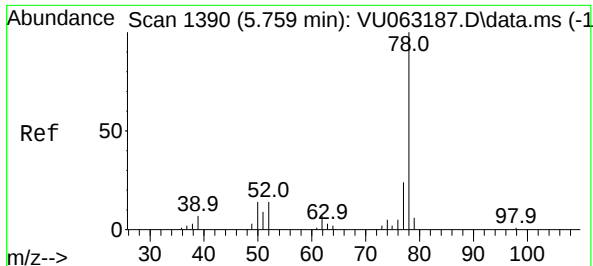

#33

Benzene

Concen: 0.135 ug/L

RT: 5.766 min Scan# 1392

Delta R.T. 0.006 min

Lab File: VU063192.D

Acq: 06 Feb 2025 13:43





Instrument :

MSVOA_U

ClientSampleId :

DCZP1DL

Tgt Ion: 78 Resp: 3611

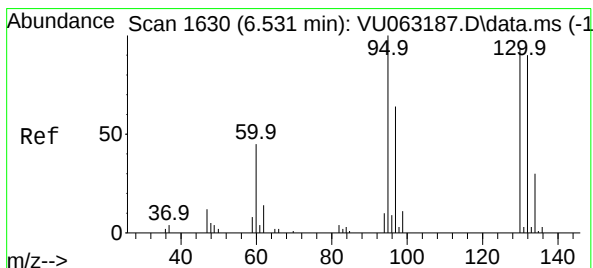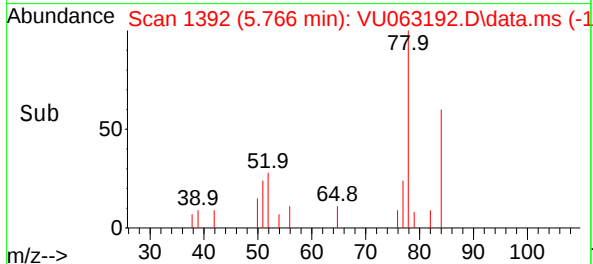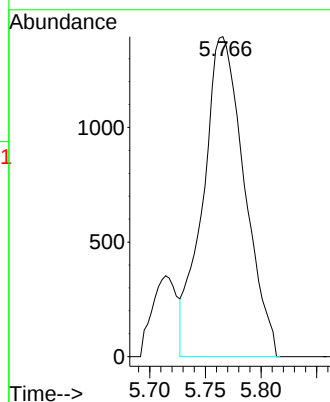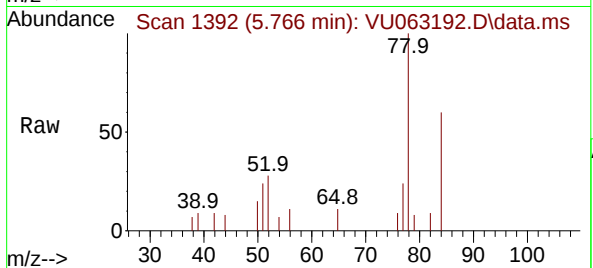

#34

Trichloroethene

Concen: 2.409 ug/L

RT: 6.531 min Scan# 1630

Delta R.T. -0.000 min

Lab File: VU063192.D

Acq: 06 Feb 2025 13:43

Tgt Ion: 95 Resp: 16323




Ion Ratio Lower Upper


95 100

97 63.5 46.7 86.7

132 91.7 62.4 115.8

130 98.0 67.3 124.9

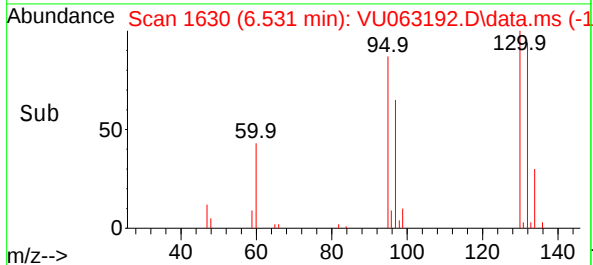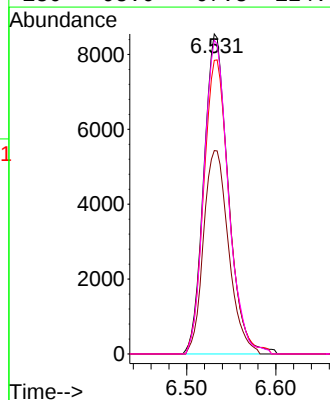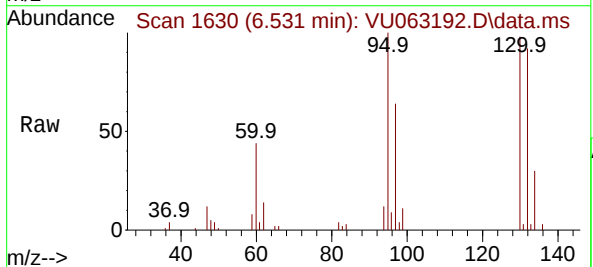

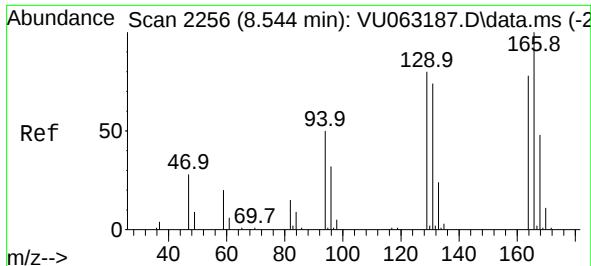

#47

Tetrachloroethene

Concen: 1.068 ug/L

RT: 8.544 min Scan# 21

Delta R.T. -0.000 min

Lab File: VU063192.D

Acq: 06 Feb 2025 13:43

Instrument :

MSVOA_U

ClientSampleId :

DCZP1DL

Tgt Ion:164 Resp: 5081





Ion Ratio Lower Upper

164 100

129 101.5 68.6 127.4

131 93.3 66.5 123.5

166 126.7 89.9 167.0

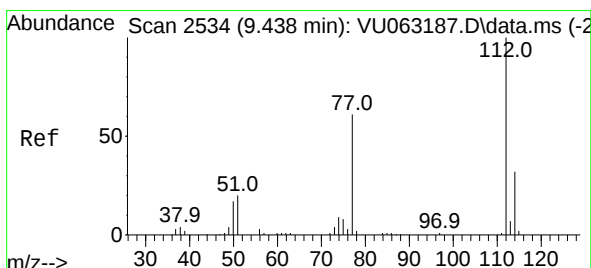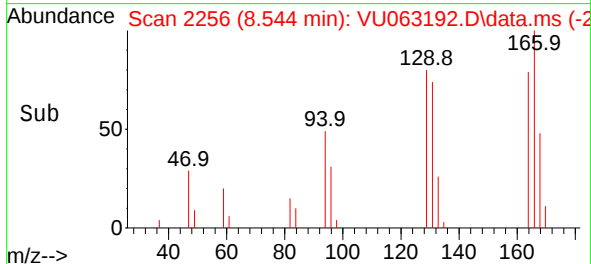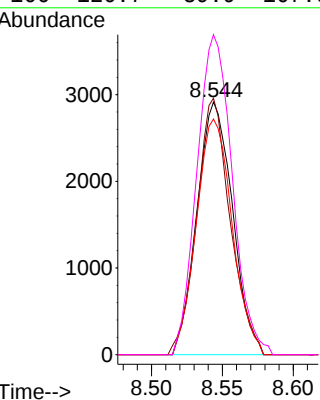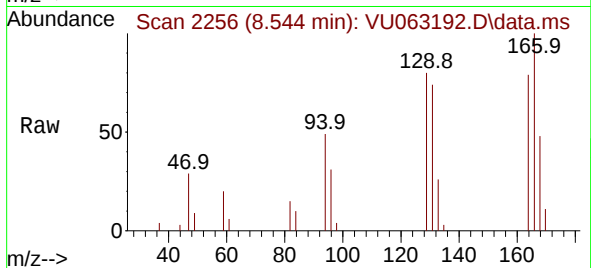

#51

Chlorobenzene

Concen: 1.645 ug/L

RT: 9.438 min Scan# 2534

Delta R.T. -0.000 min

Lab File: VU063192.D

Acq: 06 Feb 2025 13:43




Tgt Ion:112 Resp: 27689


Ion Ratio Lower Upper

112 100

114 32.1 22.6 42.0

77 61.0 50.8 76.2

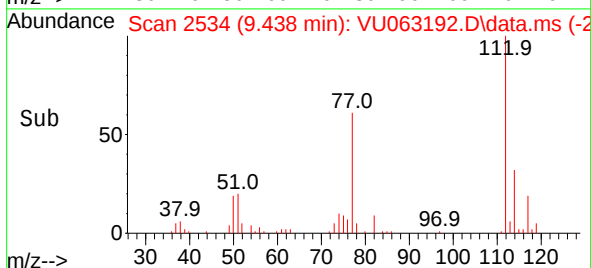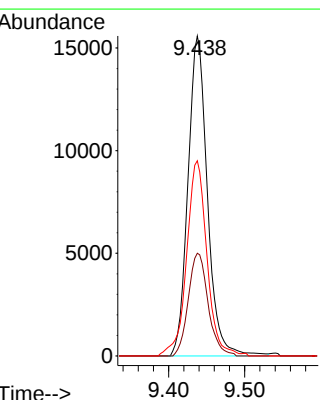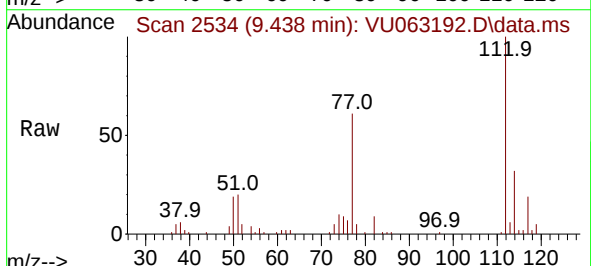

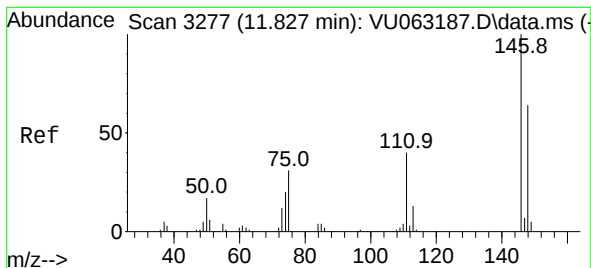

#65

1,4-Dichlorobenzene

Concen: 0.318 ug/L

RT: 11.827 min Scan# 3277

Delta R.T. -0.000 min

Lab File: VU063192.D

Acq: 06 Feb 2025 13:43

Instrument :

MSVOA_U

ClientSampleId :

DCZP1DL





Tgt Ion:146 Resp: 3290

Ion Ratio Lower Upper

146 100

111 39.3 28.5 52.9

148 64.1 45.4 84.2

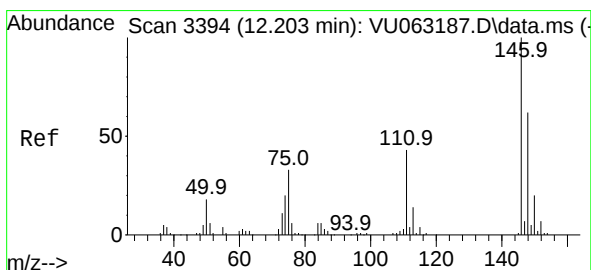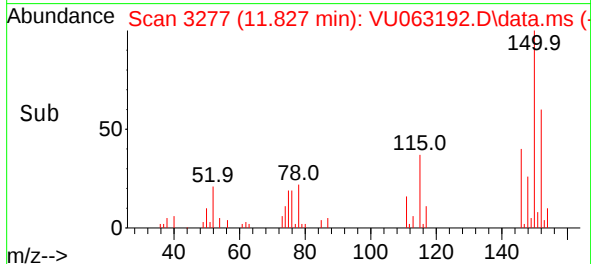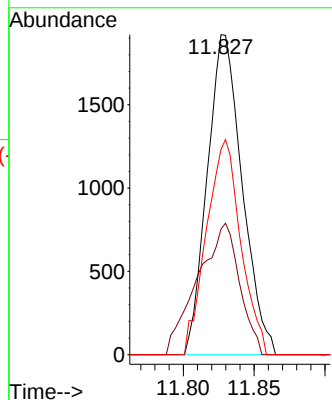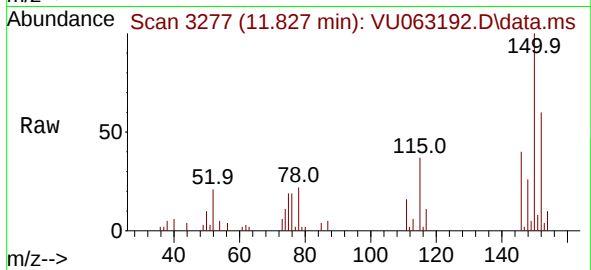

#67

1,2-Dichlorobenzene

Concen: 0.301 ug/L

RT: 12.203 min Scan# 3394

Delta R.T. -0.000 min

Lab File: VU063192.D

Acq: 06 Feb 2025 13:43

Tgt Ion:146 Resp: 2902

Ion Ratio Lower Upper

146 100

111 42.7 34.1 51.1

148 59.4 52.5 78.7

