


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020625\
Data File : VU063186.D
Acq On : 06 Feb 2025 09:57
Operator : MD/SY
Sample : BFB074
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB074

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020425WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Feb 07 07:28:28 2025

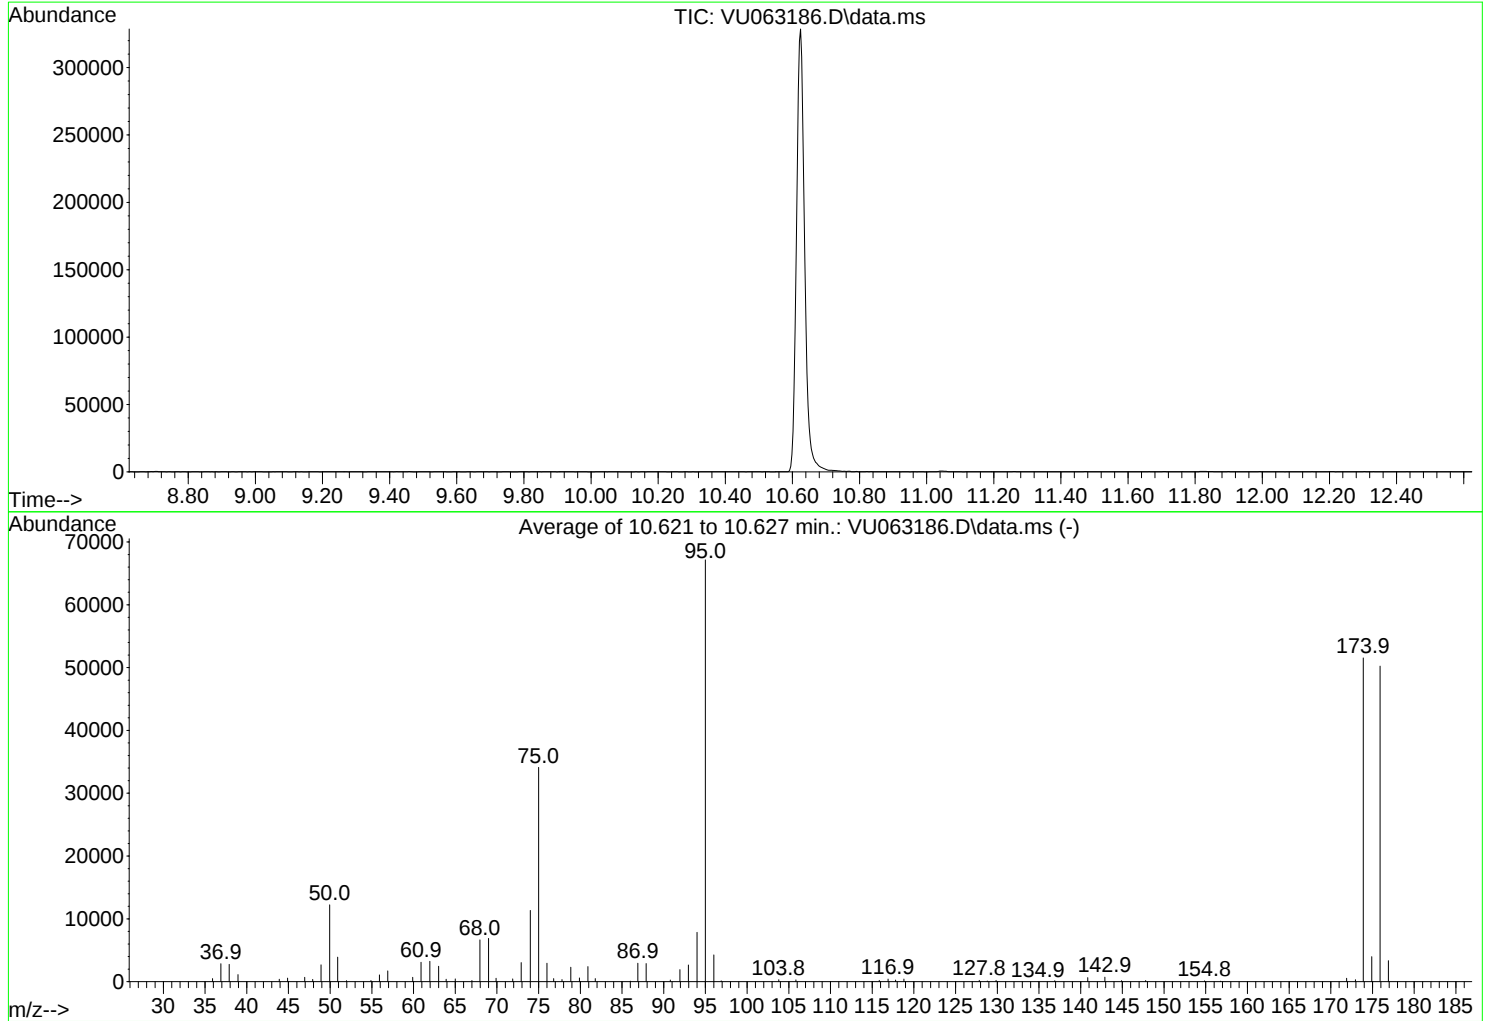

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.2	12242	PASS
75	95	30	80	50.8	34107	PASS
95	95	100	100	100.0	67163	PASS
96	95	5	9	6.3	4254	PASS
173	174	0.00	2	0.6	304	PASS
174	95	50	120	76.8	51552	PASS
175	174	5	9	7.7	3987	PASS
176	174	95	101	97.4	50237	PASS
177	176	5	9	6.6	3334	PASS

m/z	Abundance
43.90	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB074

m/z	Abundance
35.90	509.0
36.90	2879.0
37.90	2922.0
39.00	1166.0
43.90	471.0
44.90	623.0
46.90	645.0
47.90	374.0
48.90	2675.0
49.90	12484.0
50.90	4048.0
51.90	148.0
54.90	179.0
55.90	1091.0
56.90	1732.0
59.90	700.0
60.90	3303.0
62.00	3418.0
63.00	2564.0
63.90	389.0
65.00	473.0
67.00	156.0
67.90	6575.0
69.00	6934.0
69.90	545.0
71.90	437.0
72.90	3104.0
74.00	11363.0
75.00	34552.0
76.00	2937.0
76.80	502.0
77.80	319.0
78.90	2359.0
79.90	603.0
80.90	2504.0
81.80	449.0
86.90	2964.0
87.90	2877.0
90.80	275.0
92.00	1988.0
93.00	2691.0
94.00	7922.0
95.00	67808.0
96.00	4506.0
96.90	130.0
103.80	286.0
105.90	305.0
115.90	210.0
116.90	428.0
117.80	230.0
118.80	396.0
127.80	199.0
128.80	107.0
129.90	201.0
134.90	100.0
136.90	144.0
140.90	627.0
142.90	752.0
144.90	151.0
147.80	157.0
154.90	139.0
171.90	523.0
173.90	50560.0
174.90	3988.0
175.90	49296.0
176.90	3389.0

Instrument :
MSVOA_U
ClientSampleId :
BFB074

m/z	Abundance
35.90	493.0
36.90	2945.0
37.90	2836.0
39.00	1148.0
43.90	492.0
44.90	572.0
47.00	707.0
47.90	378.0
48.90	2743.0
49.90	12538.0
50.90	3993.0
52.00	154.0
54.90	193.0
55.90	1101.0
56.90	1738.0
59.90	726.0
60.90	3144.0
62.00	3334.0
63.00	2512.0
63.90	408.0
65.00	462.0
67.00	184.0
67.90	6880.0
69.00	7054.0
69.90	554.0
71.90	451.0
72.90	3140.0
74.00	11662.0
75.00	35168.0
76.00	3029.0
76.80	485.0
77.80	362.0
78.80	2352.0
79.90	580.0
80.90	2516.0
81.80	493.0
86.00	120.0
86.90	3005.0
87.90	2975.0
90.80	268.0
92.00	1985.0
93.00	2678.0
94.00	8038.0
95.00	69320.0
96.00	4347.0
96.90	128.0
103.80	316.0
105.90	290.0
115.80	194.0
116.90	419.0
117.80	266.0
118.80	437.0
127.80	207.0
128.80	108.0
129.90	221.0
136.90	152.0
140.80	670.0
142.90	712.0
144.90	169.0
147.80	186.0
154.90	146.0
156.80	106.0
171.90	571.0
173.00	462.0
173.90	53216.0
174.90	4127.0
175.90	51800.0
176.90	3430.0

Instrument :
MSVOA_U
ClientSampleId :
BFB074

m/z	Abundance
35.90	471.0
36.90	2721.0
37.90	2492.0
38.90	1045.0
43.90	475.0
44.90	506.0
47.00	696.0
47.90	348.0
48.90	2622.0
50.00	11703.0
50.90	3649.0
52.00	158.0
54.90	196.0
55.90	1010.0
56.90	1666.0
59.90	657.0
60.90	2802.0
61.90	2941.0
63.00	2296.0
63.90	368.0
65.00	403.0
67.00	176.0
68.00	6500.0
69.00	6635.0
69.90	524.0
71.90	406.0
72.90	2839.0
74.00	11023.0
75.00	32600.0
76.00	2850.0
76.80	461.0
77.80	346.0
78.80	2156.0
79.90	554.0
80.90	2203.0
81.80	501.0
86.00	119.0
86.90	2835.0
87.90	2788.0
90.80	236.0
91.90	1796.0
92.90	2568.0
94.00	7572.0
95.00	64360.0
96.00	3909.0
96.90	108.0
103.80	308.0
105.80	235.0
115.80	193.0
116.90	381.0
117.80	243.0
118.80	394.0
127.90	214.0
128.80	103.0
129.80	200.0
136.90	154.0
140.80	622.0
142.90	648.0
144.90	176.0
147.80	181.0
154.80	145.0
156.80	116.0
171.90	527.0
172.90	450.0
173.90	50880.0
174.90	3847.0
175.90	49616.0
176.90	3182.0

Instrument :
MSVOA_U
ClientSampleId :
BFB074