


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020725\
Data File : VU063211.D
Acq On : 07 Feb 2025 08:32
Operator : MD/SY
Sample : BFB075
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB075

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020425WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Feb 10 15:31:39 2025

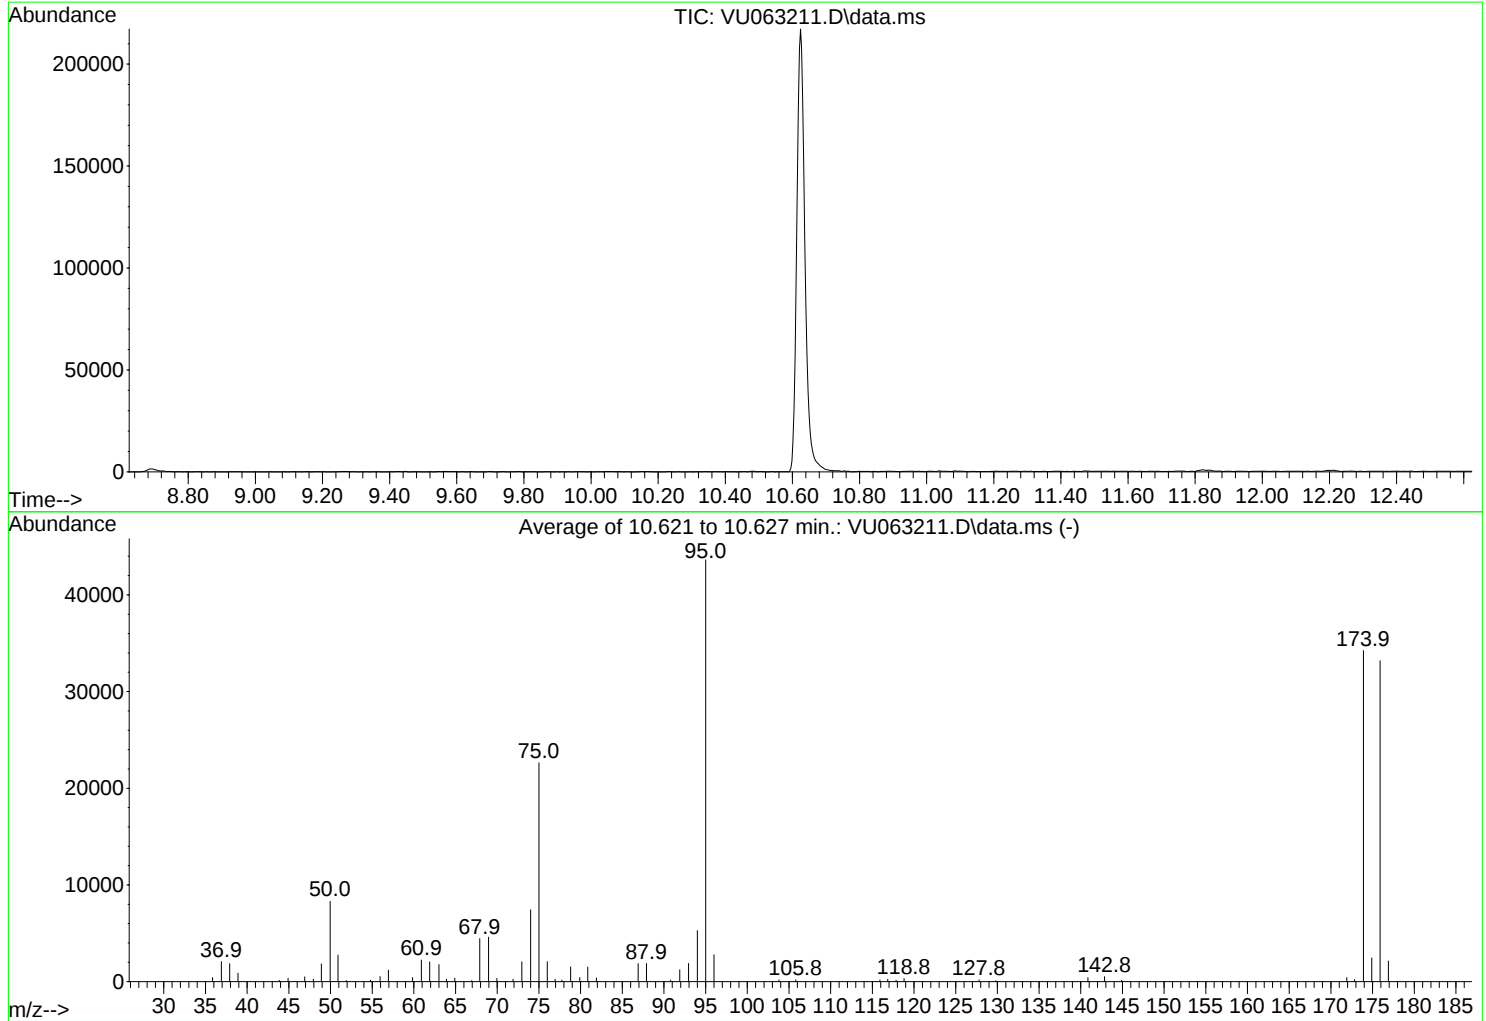

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.1	8314	PASS
75	95	30	80	51.9	22637	PASS
95	95	100	100	100.0	43629	PASS
96	95	5	9	6.4	2775	PASS
173	174	0.00	2	0.6	222	PASS
174	95	50	120	78.5	34245	PASS
175	174	5	9	7.2	2452	PASS
176	174	95	101	97.0	33205	PASS
177	176	5	9	6.4	2134	PASS

m/z	Abundance
43.80	122.0

Instrument :
MSVOA_U
ClientSampleId :
BFB075

m/z	Abundance
35.80	415.0
36.90	2003.0
37.90	1833.0
38.90	869.0
43.90	284.0
44.90	352.0
46.90	484.0
48.00	281.0
48.90	1926.0
50.00	8281.0
50.90	2704.0
51.90	116.0
54.80	133.0
55.90	549.0
56.90	1099.0
59.90	411.0
60.90	2200.0
61.90	2064.0
63.00	1742.0
63.90	234.0
64.90	353.0
66.90	111.0
67.90	4478.0
68.90	4559.0
70.00	330.0
71.90	234.0
72.90	2009.0
74.00	7360.0
75.00	22560.0
76.00	2024.0
76.90	230.0
77.80	167.0
78.80	1466.0
79.90	408.0
80.90	1545.0
81.90	357.0
86.90	1751.0
87.90	1871.0
90.80	161.0
91.90	1247.0
93.00	1887.0
94.00	5087.0
95.00	43264.0
96.00	2900.0
103.80	173.0
105.80	197.0
115.90	159.0
116.90	215.0
117.80	162.0
118.80	306.0
127.80	148.0
129.80	122.0
140.90	386.0
142.80	534.0
144.90	127.0
171.90	378.0
172.80	315.0
173.90	32896.0
174.90	2436.0
175.90	32152.0
176.90	2068.0

Instrument :
MSVOA_U
ClientSampleId :
BFB075

m/z	Abundance
35.80	417.0
36.90	2151.0
37.90	1924.0
38.90	925.0
43.90	261.0
44.90	361.0
46.90	497.0
47.90	281.0
48.90	1911.0
49.90	8539.0
50.90	2860.0
51.90	124.0
54.80	159.0
55.90	548.0
57.00	1241.0
59.90	430.0
60.90	2290.0
61.90	2070.0
63.00	1830.0
63.90	262.0
64.90	372.0
67.00	126.0
67.90	4563.0
68.90	4758.0
69.90	336.0
71.90	270.0
73.00	2123.0
74.00	7655.0
75.00	23376.0
76.00	2141.0
76.90	261.0
77.70	164.0
78.80	1571.0
79.90	454.0
80.90	1535.0
81.90	397.0
86.90	1951.0
87.90	1918.0
90.80	172.0
91.90	1251.0
93.00	1938.0
94.00	5444.0
95.00	45048.0
96.00	2844.0
103.80	186.0
105.80	200.0
115.90	172.0
116.80	254.0
117.90	159.0
118.80	326.0
127.80	195.0
129.80	104.0
140.90	435.0
142.90	533.0
144.90	139.0
171.90	438.0
173.90	35320.0
174.90	2529.0
175.90	34216.0
176.90	2210.0

Instrument :
MSVOA_U
ClientSampleId :
BFB075

m/z	Abundance
35.90	417.0
36.90	2057.0
37.90	1785.0
38.90	845.0
43.90	235.0
44.90	343.0
46.90	495.0
47.90	242.0
48.90	1697.0
49.90	8123.0
50.90	2692.0
51.90	109.0
54.80	156.0
56.00	511.0
57.00	1246.0
59.80	412.0
60.90	2198.0
61.90	1975.0
63.00	1721.0
63.90	262.0
64.90	350.0
66.90	139.0
67.90	4306.0
69.00	4482.0
69.90	339.0
71.90	236.0
73.00	2036.0
74.00	7295.0
75.00	21976.0
76.00	2024.0
77.00	276.0
77.70	175.0
78.80	1550.0
79.90	455.0
80.80	1439.0
81.90	400.0
86.90	1907.0
87.90	1827.0
90.80	174.0
91.90	1178.0
92.90	1829.0
94.00	5293.0
95.00	42576.0
96.00	2582.0
103.80	179.0
105.80	173.0
115.90	155.0
116.80	285.0
117.90	138.0
118.80	305.0
127.80	196.0
129.80	100.0
140.80	423.0
142.90	474.0
144.90	150.0
145.90	103.0
171.90	437.0
172.90	351.0
173.90	34520.0
174.90	2390.0
175.90	33248.0
176.90	2125.0

Instrument :
MSVOA_U
ClientSampleId :
BFB075