

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
 Data File : VU047080.D
 Acq On : 10 Feb 2022 17:58
 Operator : SY/MD
 Sample : VU0210WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK064

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

Signal : TIC: VU047080.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	99	rVB	286406	332886	15.31%	1.929%
2	1.919	174	180	196	rVB	206846	272059	12.51%	1.577%
3	2.575	373	384	411	rVB	461873	771969	35.51%	4.474%
4	3.446	651	655	659	rBV7	1482	1438	0.07%	0.008%
5	3.539	682	684	687	rBV4	1543	1065	0.05%	0.006%
6	3.639	712	715	725	rVB4	1570	1530	0.07%	0.009%
7	3.681	725	728	729	rBV3	730	431	0.02%	0.002%
8	3.716	735	739	742	rBV5	1050	942	0.04%	0.005%
9	3.825	770	773	775	rBV3	1014	781	0.04%	0.005%
10	3.903	791	797	798	rBV6	1141	1155	0.05%	0.007%
11	3.954	811	813	816	rVB5	1060	623	0.03%	0.004%
12	3.970	816	818	820	rBV3	857	386	0.02%	0.002%
13	4.005	827	829	831	rBV3	502	194	0.01%	0.001%
14	4.018	831	833	836	rVB4	1364	796	0.04%	0.005%
15	4.044	836	841	843	rBV6	1671	1269	0.06%	0.007%
16	4.060	844	846	848	rBV3	585	221	0.01%	0.001%
17	4.147	871	873	875	rBV3	711	348	0.02%	0.002%
18	4.189	884	886	887	rVB3	510	189	0.01%	0.001%
19	4.202	887	890	892	rBV4	1707	1335	0.06%	0.008%
20	4.243	901	903	904	rBV2	997	377	0.02%	0.002%
21	4.282	912	915	918	rVB4	1569	863	0.04%	0.005%
22	4.359	935	939	941	rBV5	898	664	0.03%	0.004%
23	4.417	956	957	960	rVB3	795	319	0.01%	0.002%
24	4.440	960	964	968	rBV7	1239	927	0.04%	0.005%
25	4.462	968	971	975	rVB6	1258	933	0.04%	0.005%
26	4.485	975	978	981	rBV4	1287	972	0.04%	0.006%
27	4.526	989	991	994	rBV3	1312	813	0.04%	0.005%
28	4.639	1012	1026	1065	rBV	214117	682810	31.41%	3.957%
29	4.973	1127	1130	1133	rVB5	1211	747	0.03%	0.004%
30	4.993	1133	1136	1138	rBV4	1356	938	0.04%	0.005%
31	5.067	1144	1159	1182	rBV	371643	812883	37.39%	4.711%
32	5.276	1222	1224	1225	rBV2	1345	612	0.03%	0.004%
33	5.433	1271	1273	1276	rBV4	1459	977	0.04%	0.006%
34	5.485	1286	1289	1292	rVB5	849	551	0.03%	0.003%
35	5.507	1293	1296	1300	rBV5	1754	1260	0.06%	0.007%
36	5.565	1308	1314	1317	rBV7	905	936	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
 Data File : VU047080.D
 Acq On : 10 Feb 2022 17:58
 Operator : SY/MD
 Sample : VU0210WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK064

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

37	5.584	1317	1320	1322	rVB4	762	407	0.02%	0.002%
38	5.603	1323	1326	1327	rBV3	971	513	0.02%	0.003%
39	5.639	1335	1337	1339	rVB3	629	214	0.01%	0.001%
40	5.729	1339	1365	1394	rBV2	805578	2173993	100.00%	12.600%
41	6.044	1460	1463	1468	rBV6	1620	1688	0.08%	0.010%
42	6.121	1484	1487	1488	rBV3	1661	920	0.04%	0.005%
43	6.169	1497	1502	1505	rBV7	1203	1152	0.05%	0.007%
44	6.253	1512	1528	1554	rBV	596368	1170958	53.86%	6.787%
45	6.693	1652	1665	1684	rBV	491524	958208	44.08%	5.554%
46	7.044	1768	1774	1782	rBV8	2716	3151	0.14%	0.018%
47	7.079	1783	1785	1787	rBV3	898	422	0.02%	0.002%
48	7.259	1838	1841	1843	rBV4	1149	649	0.03%	0.004%
49	7.311	1855	1857	1861	rVB5	914	487	0.02%	0.003%
50	7.353	1868	1870	1872	rBV3	765	412	0.02%	0.002%
51	7.427	1889	1893	1897	rBV6	2122	2408	0.11%	0.014%
52	7.481	1908	1910	1912	rVB3	1197	531	0.02%	0.003%
53	7.568	1923	1937	1956	rBV	325283	574910	26.44%	3.332%
54	7.899	2026	2040	2080	rBV	971600	1895558	87.19%	10.986%
55	8.134	2110	2113	2115	rBV4	1177	822	0.04%	0.005%
56	8.179	2115	2127	2149	rVV	225472	387764	17.84%	2.247%
57	8.488	2219	2223	2224	rBV3	961	726	0.03%	0.004%
58	8.545	2238	2241	2243	rBV3	2064	1553	0.07%	0.009%
59	8.636	2257	2269	2282	rBV	823516	1418072	65.23%	8.219%
60	9.070	2403	2404	2405	rBV	883	308	0.01%	0.002%
61	9.118	2415	2419	2426	rBV8	1177	1920	0.09%	0.011%
62	9.189	2436	2441	2442	rBV5	1363	1184	0.05%	0.007%
63	9.317	2479	2481	2484	rBV3	1007	438	0.02%	0.003%
64	9.420	2494	2513	2544	rBV	781582	1416296	65.15%	8.209%
65	9.877	2652	2655	2658	rBV5	712	378	0.02%	0.002%
66	9.893	2658	2660	2661	rBV2	539	295	0.01%	0.002%
67	10.015	2694	2698	2699	rBV4	1064	727	0.03%	0.004%
68	10.066	2712	2714	2717	rBV4	906	516	0.02%	0.003%
69	10.108	2717	2727	2743	rVB4	5309	13061	0.60%	0.076%
70	10.172	2743	2747	2748	rBV4	1394	941	0.04%	0.005%
71	10.224	2761	2763	2765	rVB3	981	478	0.02%	0.003%
72	10.295	2782	2785	2786	rBV3	960	586	0.03%	0.003%
73	10.330	2795	2796	2799	rVB3	757	336	0.02%	0.002%
74	10.352	2799	2803	2806	rBV5	1310	1170	0.05%	0.007%
75	10.378	2809	2811	2815	rBV4	1606	1076	0.05%	0.006%
76	10.401	2815	2818	2819	rBV3	1132	632	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
 Data File : VU047080.D
 Acq On : 10 Feb 2022 17:58
 Operator : SY/MD
 Sample : VU0210WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK064

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

77	10.433	2824	2828	2831	rVB7	636	488	0.02%	0.003%
78	10.462	2831	2837	2838	rBV4	2024	1815	0.08%	0.011%
79	10.590	2874	2877	2883	rVB7	1102	769	0.04%	0.004%
80	10.758	2912	2929	2946	rBV	690705	1136053	52.26%	6.584%
81	11.092	3025	3033	3037	rBV7	4333	6211	0.29%	0.036%
82	11.259	3083	3085	3087	rVB2	1105	399	0.02%	0.002%
83	11.568	3176	3181	3182	rBV5	2435	1536	0.07%	0.009%
84	11.674	3210	3214	3215	rBV3	1631	1095	0.05%	0.006%
85	11.812	3245	3257	3277	rBV	890508	1442896	66.37%	8.363%
86	12.095	3342	3345	3346	rBV3	946	575	0.03%	0.003%
87	12.192	3360	3375	3398	rBV	995825	1661660	76.43%	9.631%
88	12.504	3470	3472	3477	rBV4	1115	1028	0.05%	0.006%
89	12.558	3484	3489	3494	rBV7	1486	1915	0.09%	0.011%
90	12.626	3507	3510	3512	rBV4	2037	1284	0.06%	0.007%
91	12.722	3537	3540	3543	rBV5	1585	1418	0.07%	0.008%
92	13.118	3660	3663	3664	rBV3	1518	953	0.04%	0.006%
93	13.224	3686	3696	3708	rBV5	7866	14636	0.67%	0.085%
94	13.417	3753	3756	3757	rBV3	1224	705	0.03%	0.004%
95	13.757	3859	3862	3865	rVB4	1877	1257	0.06%	0.007%
96	13.780	3866	3869	3872	rVV4	1161	729	0.03%	0.004%
97	13.841	3881	3888	3902	rVB3	11533	19795	0.91%	0.115%
98	14.150	3980	3984	3988	rBV7	1572	1739	0.08%	0.010%
99	14.198	3995	3999	4000	rBV4	1300	1073	0.05%	0.006%
100	14.333	4030	4041	4051	rBV5	10707	20731	0.95%	0.120%




Sum of corrected areas: 17253819

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
Data File : VU047080.D
Acq On : 10 Feb 2022 17:58
Operator : SY/MD
Sample : VU0210WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK064

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

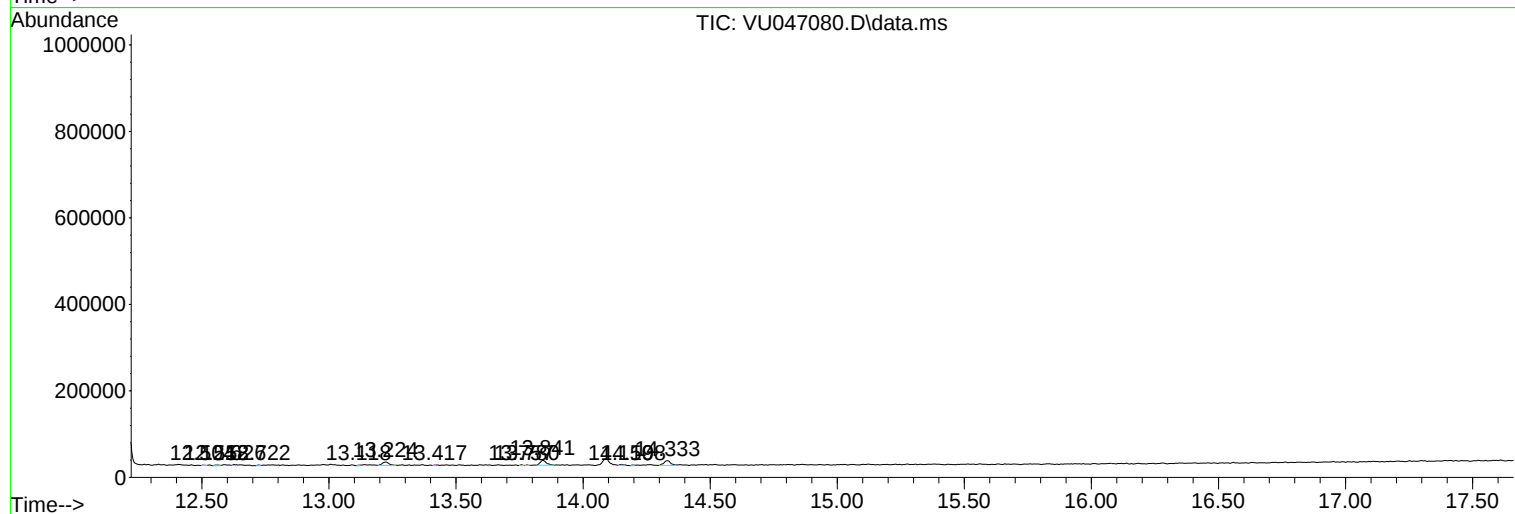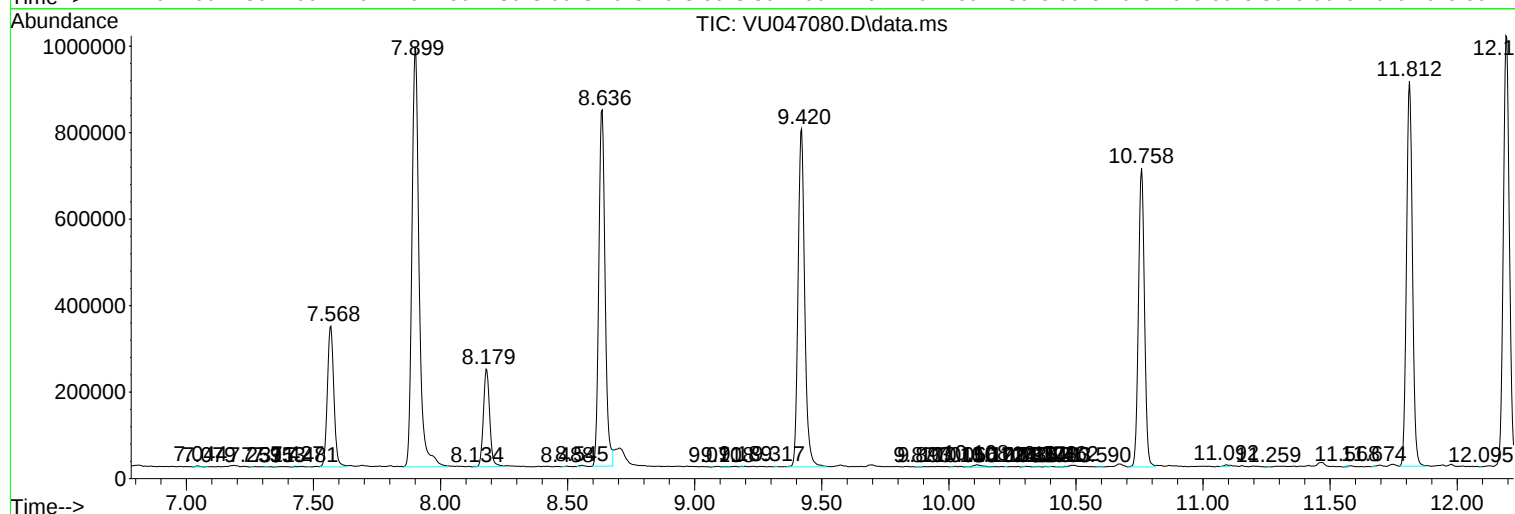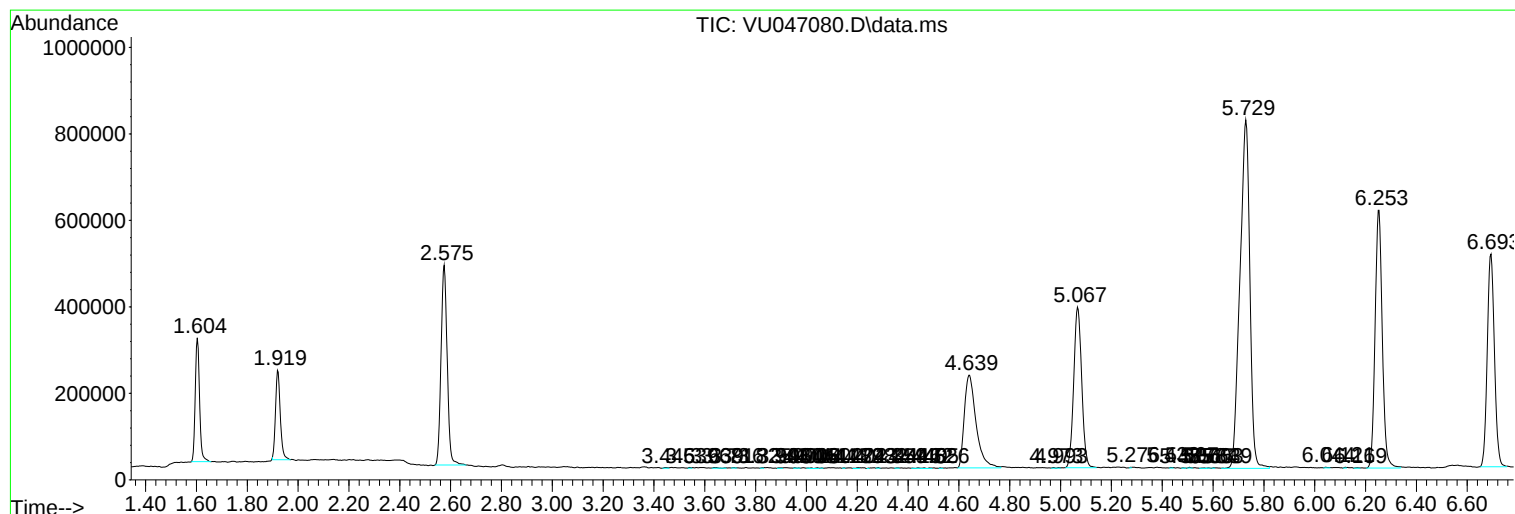

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
Data File : VU047080.D
Acq On : 10 Feb 2022 17:58
Operator : SY/MD
Sample : VU0210WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK064

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
Data File : VU047080.D
Acq On : 10 Feb 2022 17:58
Operator : SY/MD
Sample : VU0210WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK064

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------