

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
 Data File : VU047081.D
 Acq On : 10 Feb 2022 18:20
 Operator : SY/MD
 Sample : N1474-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

Signal : TIC: VU047081.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	99	rBV	276768	322846	15.60%	1.951%
2	1.919	174	180	197	rVB	199674	264628	12.79%	1.599%
3	2.575	373	384	408	rBV	447851	750839	36.28%	4.538%
4	3.144	557	561	564	rBV5	2035	1527	0.07%	0.009%
5	3.607	700	705	706	rBV5	1734	1177	0.06%	0.007%
6	3.803	764	766	773	rVB8	1344	1112	0.05%	0.007%
7	3.835	773	776	778	rBV4	1596	1249	0.06%	0.008%
8	3.935	805	807	809	rVB3	700	242	0.01%	0.001%
9	3.954	809	813	816	rBV5	1205	981	0.05%	0.006%
10	4.002	823	828	829	rBV4	1606	1444	0.07%	0.009%
11	4.041	838	840	841	rVB2	767	221	0.01%	0.001%
12	4.080	850	852	854	rBV3	1041	568	0.03%	0.003%
13	4.215	892	894	897	rBV4	962	471	0.02%	0.003%
14	4.285	913	916	917	rBV3	778	420	0.02%	0.003%
15	4.346	928	935	936	rBV6	1230	1290	0.06%	0.008%
16	4.356	936	938	941	rBV4	750	429	0.02%	0.003%
17	4.404	950	953	956	rBV4	1311	1055	0.05%	0.006%
18	4.456	959	969	973	rBV4	1680	2602	0.13%	0.016%
19	4.546	994	997	999	rBV4	1009	579	0.03%	0.003%
20	4.578	1004	1007	1010	rBV5	1814	1340	0.06%	0.008%
21	4.639	1012	1026	1054	rBV	220389	672273	32.49%	4.063%
22	5.067	1146	1159	1183	rVB	374749	822199	39.73%	4.969%
23	5.433	1270	1273	1279	rBV8	1011	881	0.04%	0.005%
24	5.478	1285	1287	1291	rVB5	1073	526	0.03%	0.003%
25	5.501	1291	1294	1295	rBV3	1297	627	0.03%	0.004%
26	5.562	1310	1313	1316	rVB5	1967	1461	0.07%	0.009%
27	5.578	1316	1318	1319	rBV2	148	56	0.00%	0.000%
28	5.594	1319	1323	1327	rBV8	1071	851	0.04%	0.005%
29	5.613	1327	1329	1331	rBV3	475	287	0.01%	0.002%
30	5.729	1344	1365	1388	rBV2	770819	2069348	100.00%	12.506%
31	6.141	1491	1493	1498	rBV6	1364	1032	0.05%	0.006%
32	6.176	1502	1504	1506	rBV3	982	499	0.02%	0.003%
33	6.195	1508	1510	1513	rBV3	648	500	0.02%	0.003%
34	6.253	1513	1528	1552	rBV	557856	1096063	52.97%	6.624%
35	6.694	1652	1665	1685	rBV	465526	914333	44.18%	5.526%
36	6.896	1726	1728	1729	rBV2	1012	533	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
 Data File : VU047081.D
 Acq On : 10 Feb 2022 18:20
 Operator : SY/MD
 Sample : N1474-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

37	6.964	1746	1749	1751	rBV3	1248	905	0.04%	0.005%
38	7.012	1762	1764	1765	rBV2	854	386	0.02%	0.002%
39	7.173	1805	1814	1816	rBV8	3211	3677	0.18%	0.022%
40	7.285	1844	1849	1851	rBV5	1046	740	0.04%	0.004%
41	7.304	1851	1855	1858	rVV5	1125	913	0.04%	0.006%
42	7.346	1863	1868	1870	rBV5	1485	989	0.05%	0.006%
43	7.362	1870	1873	1874	rBV3	707	327	0.02%	0.002%
44	7.446	1896	1899	1903	rVB6	1947	1541	0.07%	0.009%
45	7.478	1903	1909	1912	rBV7	1733	1578	0.08%	0.010%
46	7.568	1921	1937	1955	rBV	312436	557597	26.95%	3.370%
47	7.764	1996	1998	1999	rBV2	809	323	0.02%	0.002%
48	7.899	2027	2040	2058	rBV	937516	1769169	85.49%	10.692%
49	8.105	2101	2104	2107	rVB5	1180	788	0.04%	0.005%
50	8.131	2107	2112	2115	rBV7	1609	1370	0.07%	0.008%
51	8.179	2115	2127	2154	rVV	217437	376269	18.18%	2.274%
52	8.349	2178	2180	2186	rVB5	1690	1554	0.08%	0.009%
53	8.375	2186	2188	2191	rBV4	788	532	0.03%	0.003%
54	8.391	2191	2193	2195	rBV4	1304	772	0.04%	0.005%
55	8.472	2210	2218	2232	rVB	42924	77669	3.75%	0.469%
56	8.636	2256	2269	2284	rBV	781097	1367921	66.10%	8.267%
57	8.874	2340	2343	2347	rBV5	1669	1422	0.07%	0.009%
58	9.031	2387	2392	2395	rBV6	919	919	0.04%	0.006%
59	9.089	2408	2410	2413	rBV4	769	482	0.02%	0.003%
60	9.169	2427	2435	2439	rBV8	1916	2909	0.14%	0.018%
61	9.279	2467	2469	2473	rBV4	1272	936	0.05%	0.006%
62	9.359	2491	2494	2497	rBV5	1047	947	0.05%	0.006%
63	9.420	2500	2513	2538	rVV	735564	1324991	64.03%	8.007%
64	9.803	2628	2632	2637	rVB5	1731	1985	0.10%	0.012%
65	9.828	2637	2640	2643	rBV5	651	459	0.02%	0.003%
66	9.848	2643	2646	2648	rBV4	1180	807	0.04%	0.005%
67	9.861	2648	2650	2654	rVB4	1154	636	0.03%	0.004%
68	9.909	2663	2665	2670	rBV5	1209	945	0.05%	0.006%
69	10.018	2693	2699	2703	rBV8	1739	2027	0.10%	0.012%
70	10.070	2712	2715	2717	rVB4	775	340	0.02%	0.002%
71	10.105	2719	2726	2735	rBV4	5398	10989	0.53%	0.066%
72	10.288	2781	2783	2784	rBV2	1145	470	0.02%	0.003%
73	10.359	2802	2805	2811	rVB5	1475	1246	0.06%	0.008%
74	10.427	2823	2826	2829	rBV5	1216	1032	0.05%	0.006%
75	10.758	2915	2929	2945	rBV	666961	1090601	52.70%	6.591%
76	11.086	3027	3031	3033	rBV4	3526	3024	0.15%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
 Data File : VU047081.D
 Acq On : 10 Feb 2022 18:20
 Operator : SY/MD
 Sample : N1474-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

77	11.201	3065	3067	3068	rBV2	1190	531	0.03%	0.003%
78	11.269	3086	3088	3090	rBV3	805	440	0.02%	0.003%
79	11.365	3113	3118	3121	rBV7	1741	1706	0.08%	0.010%
80	11.468	3140	3150	3159	rBV3	10073	18497	0.89%	0.112%
81	11.584	3178	3186	3189	rBV9	3033	3762	0.18%	0.023%
82	11.642	3200	3204	3206	rBV5	1473	1240	0.06%	0.007%
83	11.693	3216	3220	3227	rVB7	3261	4319	0.21%	0.026%
84	11.812	3244	3257	3278	rBV	838490	1354209	65.44%	8.184%
85	12.031	3323	3325	3328	rBV3	1816	1264	0.06%	0.008%
86	12.192	3363	3375	3392	rVB	960940	1585997	76.64%	9.585%
87	12.430	3446	3449	3452	rVB5	1191	787	0.04%	0.005%
88	12.520	3475	3477	3479	rBV2	724	374	0.02%	0.002%
89	12.867	3581	3585	3587	rBV5	1252	1127	0.05%	0.007%
90	13.066	3643	3647	3649	rBV5	1548	1214	0.06%	0.007%
91	13.147	3667	3672	3674	rBV6	1526	1587	0.08%	0.010%
92	13.459	3765	3769	3770	rBV3	1166	844	0.04%	0.005%
93	13.754	3857	3861	3864	rBV6	1011	869	0.04%	0.005%
94	13.812	3877	3879	3880	rBV3	724	267	0.01%	0.002%
95	13.893	3902	3904	3905	rBV2	1110	538	0.03%	0.003%
96	14.089	3958	3965	3974	rVB2	11231	17644	0.85%	0.107%
97	14.455	4076	4079	4080	rBV3	1249	767	0.04%	0.005%
98	14.629	4130	4133	4136	rBV5	1120	702	0.03%	0.004%




Sum of corrected areas: 16547361

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
Data File : VU047081.D
Acq On : 10 Feb 2022 18:20
Operator : SY/MD
Sample : N1474-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

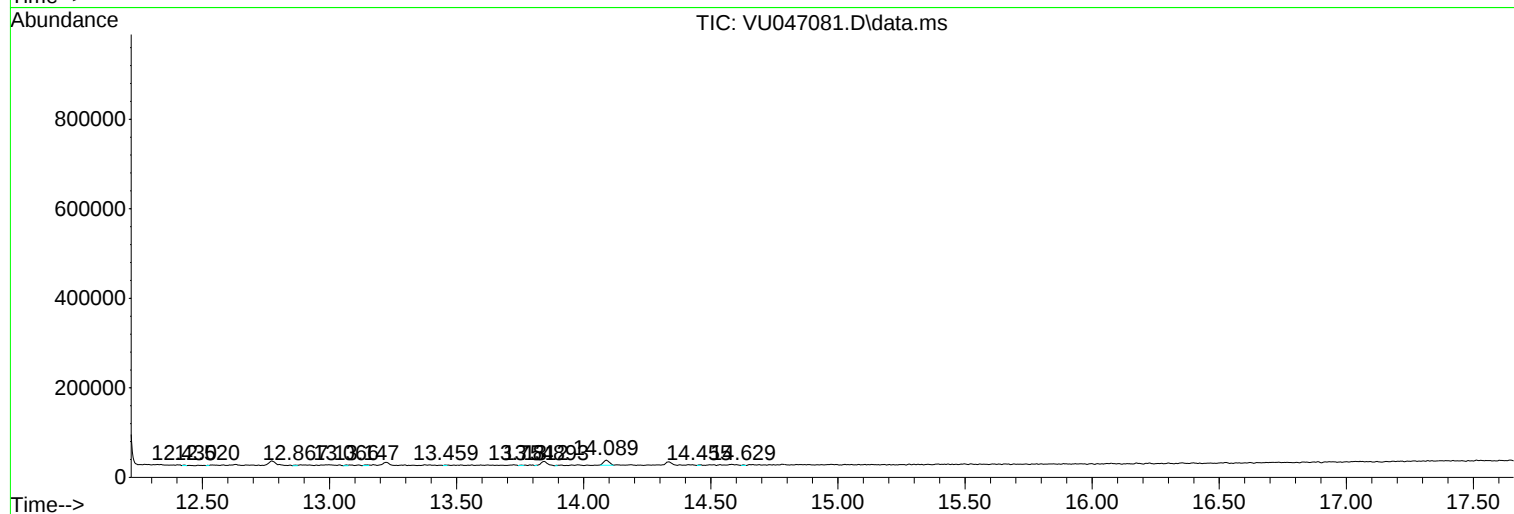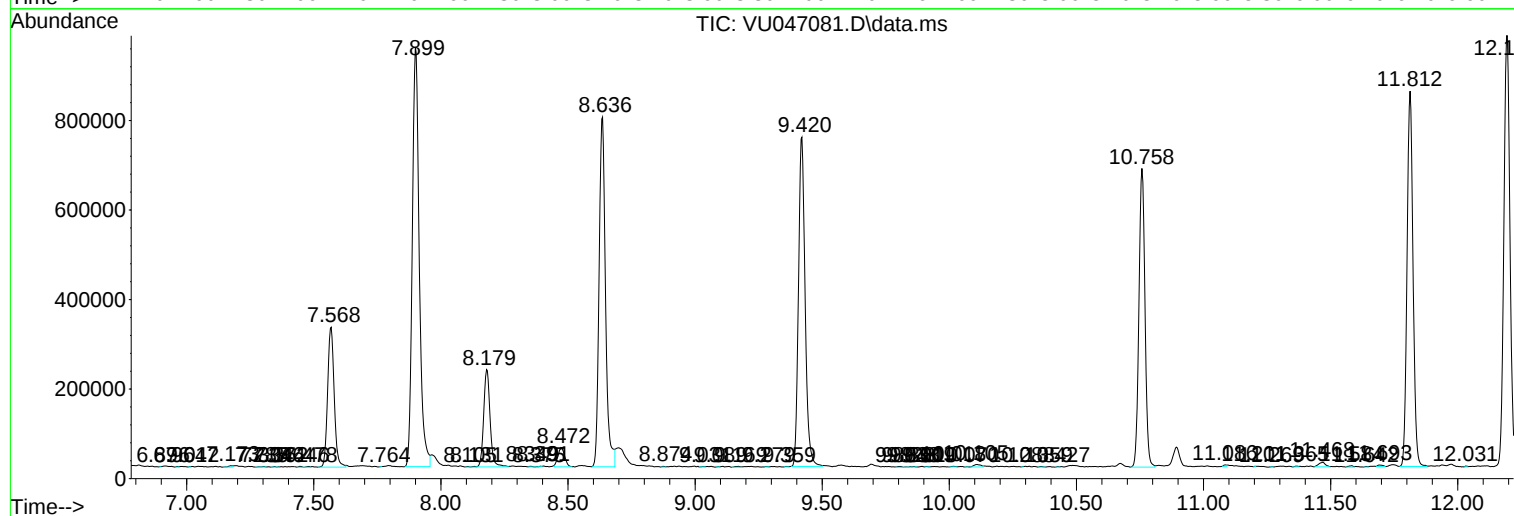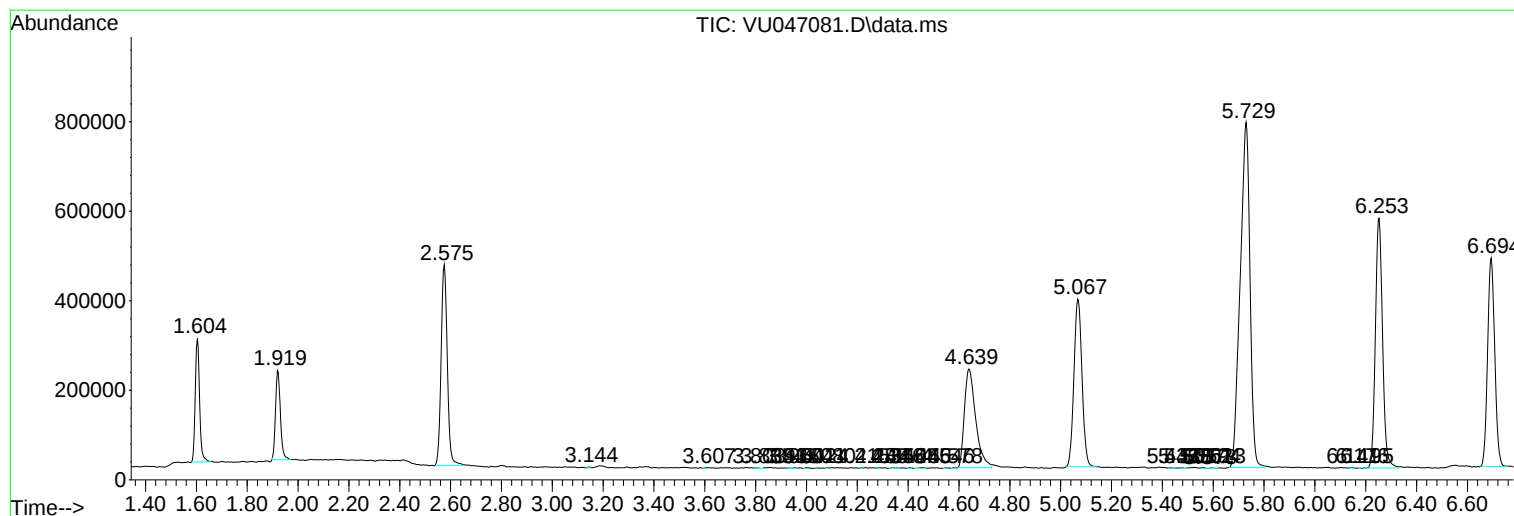

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
Data File : VU047081.D
Acq On : 10 Feb 2022 18:20
Operator : SY/MD
Sample : N1474-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
Data File : VU047081.D
Acq On : 10 Feb 2022 18:20
Operator : SY/MD
Sample : N1474-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc