

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
 Data File : VU047093.D
 Acq On : 10 Feb 2022 22:53
 Operator : SY/MD
 Sample : N1462-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M49

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

Signal : TIC: VU047093.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	99	rVB	253749	294237	14.74%	1.856%
2	1.922	174	181	197	rVB	183032	243556	12.20%	1.537%
3	2.575	374	384	404	rBV	413286	672798	33.71%	4.245%
4	3.141	556	560	563	rBV4	1423	1314	0.07%	0.008%
5	3.289	602	606	610	rBV4	1916	1732	0.09%	0.011%
6	3.472	659	663	666	rBV6	1704	1259	0.06%	0.008%
7	3.501	670	672	674	rBV2	999	576	0.03%	0.004%
8	3.620	706	709	710	rBV3	547	310	0.02%	0.002%
9	3.629	710	712	716	rVB4	1451	829	0.04%	0.005%
10	3.735	743	745	747	rBV3	1430	818	0.04%	0.005%
11	3.809	765	768	771	rBV5	1401	1154	0.06%	0.007%
12	3.854	780	782	786	rBV5	1133	979	0.05%	0.006%
13	3.877	786	789	793	rVV4	1182	1084	0.05%	0.007%
14	3.916	798	801	803	rBV3	1037	631	0.03%	0.004%
15	3.932	804	806	811	rVB4	1204	942	0.05%	0.006%
16	3.964	811	816	819	rBV8	1724	1512	0.08%	0.010%
17	4.009	829	830	835	rVB5	1198	833	0.04%	0.005%
18	4.054	841	844	847	rBV5	1015	800	0.04%	0.005%
19	4.099	856	858	861	rBV4	673	366	0.02%	0.002%
20	4.128	865	867	871	rVB6	590	375	0.02%	0.002%
21	4.150	873	874	875	rBV	482	101	0.01%	0.001%
22	4.176	880	882	884	rBV3	1287	817	0.04%	0.005%
23	4.215	890	894	899	rVB5	2021	1608	0.08%	0.010%
24	4.240	899	902	903	rBV3	440	287	0.01%	0.002%
25	4.324	925	928	929	rBV3	834	417	0.02%	0.003%
26	4.334	929	931	932	rVV2	498	201	0.01%	0.001%
27	4.362	937	940	941	rBV3	677	380	0.02%	0.002%
28	4.404	949	953	954	rBV4	1296	809	0.04%	0.005%
29	4.465	970	972	974	rBV3	654	365	0.02%	0.002%
30	4.488	976	979	983	rVV6	831	722	0.04%	0.005%
31	4.539	988	995	998	rBV6	1427	2063	0.10%	0.013%
32	4.578	1003	1007	1009	rBV4	1235	790	0.04%	0.005%
33	4.591	1009	1011	1012	rBV2	1184	480	0.02%	0.003%
34	4.645	1013	1028	1071	rBV2	185754	664707	33.30%	4.194%
35	4.867	1094	1097	1100	rBV5	1543	1131	0.06%	0.007%
36	5.067	1144	1159	1182	rBV	339168	748454	37.50%	4.722%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
 Data File : VU047093.D
 Acq On : 10 Feb 2022 22:53
 Operator : SY/MD
 Sample : N1462-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M49

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

37	5.449	1275	1278	1281	rBV5	1229	966	0.05%	0.006%
38	5.494	1289	1292	1295	rVB4	901	685	0.03%	0.004%
39	5.514	1295	1298	1303	rBV6	1788	1991	0.10%	0.013%
40	5.542	1303	1307	1309	rBV5	1223	923	0.05%	0.006%
41	5.629	1331	1334	1337	rVB4	1062	610	0.03%	0.004%
42	5.729	1337	1365	1388	rBV2	736353	1995850	100.00%	12.592%
43	6.253	1512	1528	1554	rBV	551517	1088833	54.55%	6.869%
44	6.539	1608	1617	1622	rBV	4311	8215	0.41%	0.052%
45	6.694	1653	1665	1685	rVB	453799	878168	44.00%	5.540%
46	6.996	1755	1759	1760	rBV4	1005	627	0.03%	0.004%
47	7.137	1801	1803	1806	rVB4	1279	536	0.03%	0.003%
48	7.321	1855	1860	1862	rBV6	709	599	0.03%	0.004%
49	7.333	1862	1864	1865	rBV2	704	303	0.02%	0.002%
50	7.349	1865	1869	1873	rBV7	1177	1177	0.06%	0.007%
51	7.449	1896	1900	1901	rBV4	1662	953	0.05%	0.006%
52	7.472	1905	1907	1909	rBV3	844	474	0.02%	0.003%
53	7.501	1913	1916	1920	rBV7	1684	1322	0.07%	0.008%
54	7.568	1924	1937	1951	rBV	296684	519366	26.02%	3.277%
55	7.841	2020	2022	2024	rBV3	1160	677	0.03%	0.004%
56	7.899	2027	2040	2075	rVV	889899	1729460	86.65%	10.911%
57	8.179	2116	2127	2149	rBV	204666	350112	17.54%	2.209%
58	8.636	2257	2269	2284	rBV	770715	1360381	68.16%	8.583%
59	8.886	2345	2347	2349	rBV3	1382	826	0.04%	0.005%
60	8.954	2365	2368	2371	rBV4	1821	969	0.05%	0.006%
61	8.992	2378	2380	2384	rVB4	947	529	0.03%	0.003%
62	9.108	2413	2416	2419	rBV5	1553	1101	0.06%	0.007%
63	9.185	2436	2440	2442	rBV5	1416	1178	0.06%	0.007%
64	9.295	2472	2474	2477	rBV3	1494	975	0.05%	0.006%
65	9.420	2500	2513	2538	rBV	734401	1312276	65.75%	8.279%
66	9.697	2592	2599	2602	rBV7	2726	3638	0.18%	0.023%
67	9.787	2624	2627	2633	rVB8	1778	1590	0.08%	0.010%
68	9.812	2633	2635	2636	rBV2	923	472	0.02%	0.003%
69	9.822	2636	2638	2640	rBV3	745	306	0.02%	0.002%
70	9.893	2658	2660	2662	rBV3	627	299	0.01%	0.002%
71	10.185	2749	2751	2753	rBV4	1069	541	0.03%	0.003%
72	10.285	2779	2782	2787	rVB6	1496	900	0.05%	0.006%
73	10.327	2789	2795	2799	rBV7	1113	1269	0.06%	0.008%
74	10.349	2799	2802	2805	rBV4	1250	769	0.04%	0.005%
75	10.591	2874	2877	2881	rBV7	844	914	0.05%	0.006%
76	10.671	2897	2902	2909	rVB2	5806	7770	0.39%	0.049%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
 Data File : VU047093.D
 Acq On : 10 Feb 2022 22:53
 Operator : SY/MD
 Sample : N1462-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M49

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M

Title : VOC Analysis

77	10.758	2916	2929	2948	rBV	647851	1057676	52.99%	6.673%
78	11.198	3062	3066	3076	rBV	1905	2647	0.13%	0.017%
79	11.359	3112	3116	3122	rBV8	2067	2439	0.12%	0.015%
80	11.812	3245	3257	3273	rBV	826769	1331294	66.70%	8.399%
81	12.195	3364	3376	3393	rVB	924832	1526041	76.46%	9.628%
82	13.124	3662	3665	3666	rBV3	1422	831	0.04%	0.005%
83	13.494	3778	3780	3783	rBV4	981	503	0.03%	0.003%
84	13.568	3801	3803	3806	rBV3	1427	834	0.04%	0.005%




Sum of corrected areas: 15850252

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
Data File : VU047093.D
Acq On : 10 Feb 2022 22:53
Operator : SY/MD
Sample : N1462-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

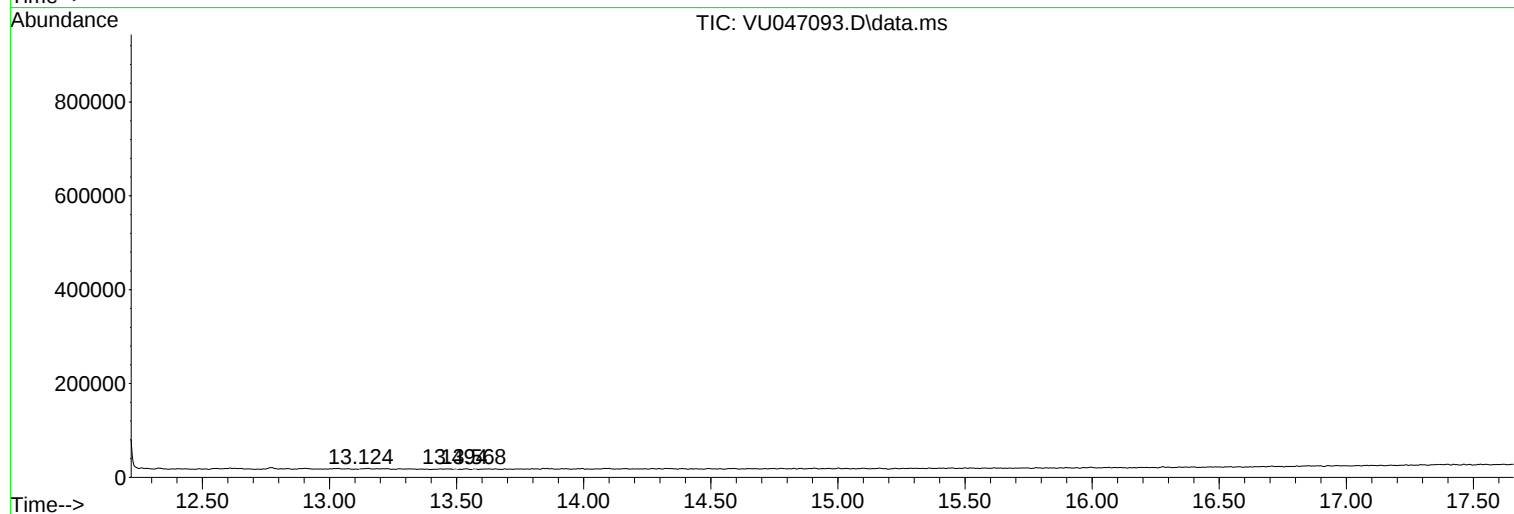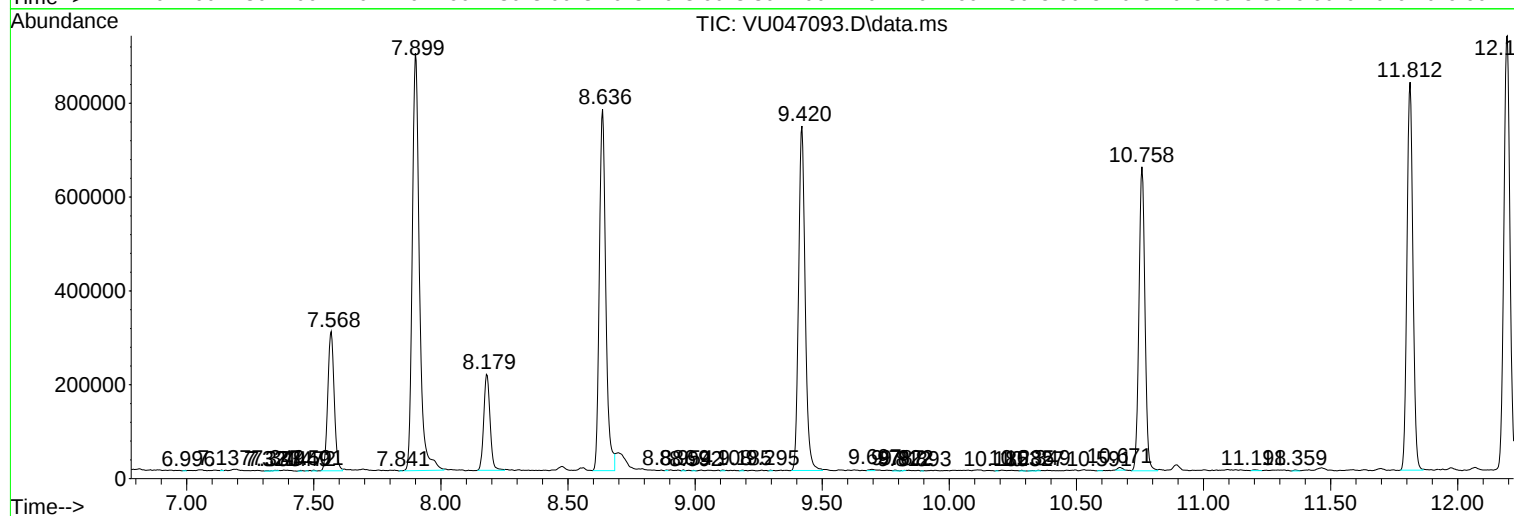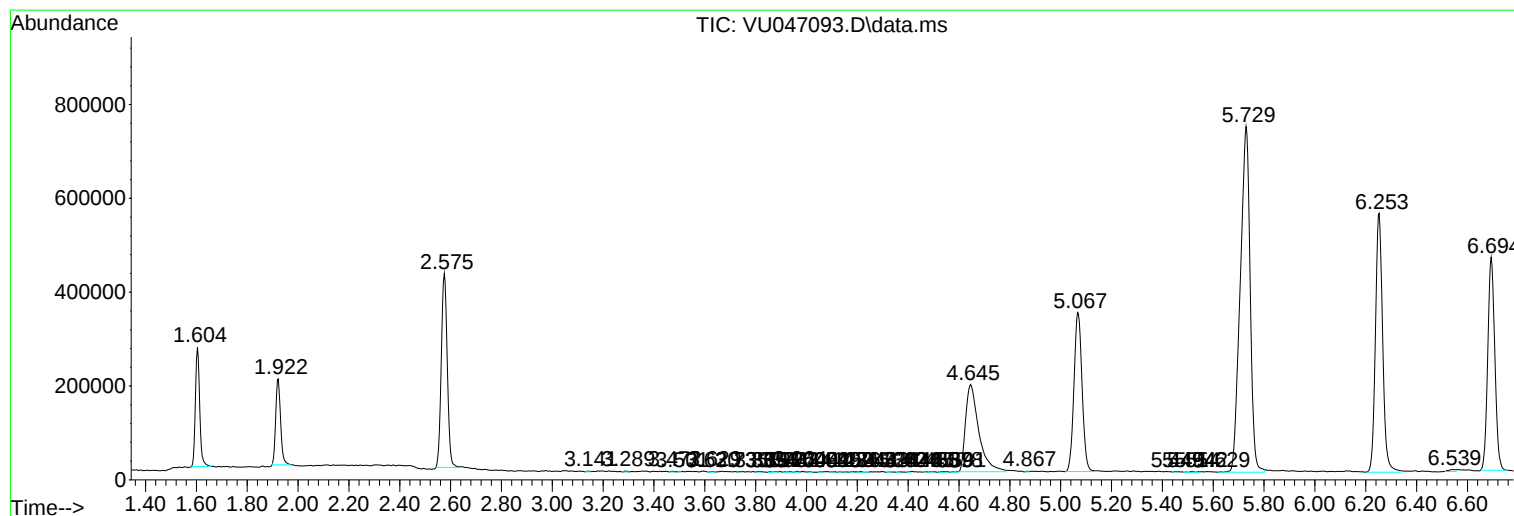

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
Data File : VU047093.D
Acq On : 10 Feb 2022 22:53
Operator : SY/MD
Sample : N1462-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
Data File : VU047093.D
Acq On : 10 Feb 2022 22:53
Operator : SY/MD
Sample : N1462-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M49

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------