

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
 Data File : VU047100.D
 Acq On : 11 Feb 2022 01:32
 Operator : SY/MD
 Sample : N1462-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

Signal : TIC: VU047100.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	101	rVB	235275	276391	14.38%	1.749%
2	1.922	174	181	197	rVB	177602	238962	12.43%	1.512%
3	2.575	374	384	400	rBV	290471	477592	24.85%	3.023%
4	3.247	591	593	597	rVB5	1713	1082	0.06%	0.007%
5	3.266	597	599	601	rBV3	845	372	0.02%	0.002%
6	3.327	614	618	619	rBV5	937	605	0.03%	0.004%
7	3.549	684	687	692	rBV6	1721	1659	0.09%	0.011%
8	3.588	697	699	704	rVB5	978	572	0.03%	0.004%
9	3.613	704	707	710	rBV4	1971	1577	0.08%	0.010%
10	3.684	725	729	730	rBV4	998	714	0.04%	0.005%
11	3.765	753	754	756	rBV3	796	381	0.02%	0.002%
12	3.864	778	785	787	rBV8	981	1067	0.06%	0.007%
13	3.919	798	802	803	rBV4	440	287	0.01%	0.002%
14	4.051	840	843	846	rBV5	1391	992	0.05%	0.006%
15	4.067	846	848	851	rVB4	1024	491	0.03%	0.003%
16	4.096	853	857	862	rBV6	1204	1163	0.06%	0.007%
17	4.115	862	863	865	rVB2	745	174	0.01%	0.001%
18	4.134	865	869	874	rVB6	1018	962	0.05%	0.006%
19	4.154	874	875	876	rBV	479	179	0.01%	0.001%
20	4.163	876	878	879	rBV2	770	299	0.02%	0.002%
21	4.218	893	895	898	rVB4	742	315	0.02%	0.002%
22	4.234	898	900	905	rBV6	1158	847	0.04%	0.005%
23	4.279	911	914	917	rBV6	1082	655	0.03%	0.004%
24	4.330	925	930	934	rVB7	1089	1074	0.06%	0.007%
25	4.379	942	945	950	rBV6	929	1084	0.06%	0.007%
26	4.440	961	964	969	rVB6	1219	1004	0.05%	0.006%
27	4.472	969	974	978	rBV6	1408	1559	0.08%	0.010%
28	4.510	984	986	989	rBV4	775	408	0.02%	0.003%
29	4.588	1008	1010	1012	rBV3	636	275	0.01%	0.002%
30	4.652	1012	1030	1074	rBV	160854	681656	35.47%	4.314%
31	5.067	1145	1159	1178	rBV	327312	718173	37.37%	4.545%
32	5.465	1280	1283	1287	rBV5	809	539	0.03%	0.003%
33	5.520	1296	1300	1304	rBV6	1965	1817	0.09%	0.012%
34	5.729	1342	1365	1393	rBV2	712393	1921988	100.00%	12.165%
35	6.253	1513	1528	1564	rBV	535779	1069631	55.65%	6.770%
36	6.465	1591	1594	1600	rVB6	1881	1782	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
 Data File : VU047100.D
 Acq On : 11 Feb 2022 01:32
 Operator : SY/MD
 Sample : N1462-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

37	6.546	1607	1619	1635	rBV2	27108	59281	3.08%	0.375%
38	6.694	1652	1665	1690	rVB	442957	862809	44.89%	5.461%
39	6.999	1753	1760	1761	rBV7	1200	1156	0.06%	0.007%
40	7.147	1801	1806	1808	rBV5	1248	1246	0.06%	0.008%
41	7.160	1808	1810	1812	rVV3	992	601	0.03%	0.004%
42	7.186	1812	1818	1827	rVB3	3035	5490	0.29%	0.035%
43	7.308	1851	1856	1857	rBV4	926	594	0.03%	0.004%
44	7.388	1878	1881	1882	rBV2	456	268	0.01%	0.002%
45	7.398	1882	1884	1886	rVB3	577	171	0.01%	0.001%
46	7.440	1895	1897	1902	rBV3	1241	902	0.05%	0.006%
47	7.469	1904	1906	1908	rVV3	477	211	0.01%	0.001%
48	7.504	1914	1917	1919	rBV3	1102	631	0.03%	0.004%
49	7.568	1924	1937	1954	rVV	277233	487888	25.38%	3.088%
50	7.745	1989	1992	1993	rBV3	1108	580	0.03%	0.004%
51	7.813	2010	2013	2017	rBV5	854	798	0.04%	0.005%
52	7.899	2027	2040	2060	rBV	851874	1613494	83.95%	10.212%
53	8.118	2104	2108	2109	rBV3	671	480	0.02%	0.003%
54	8.182	2117	2128	2142	rBV	197377	333665	17.36%	2.112%
55	8.372	2181	2187	2189	rBV7	1361	1283	0.07%	0.008%
56	8.555	2230	2244	2258	rBV	348795	616903	32.10%	3.904%
57	8.636	2259	2269	2286	rBV	717390	1277245	66.45%	8.084%
58	9.034	2391	2393	2396	rVB3	998	511	0.03%	0.003%
59	9.054	2396	2399	2401	rBV4	1448	813	0.04%	0.005%
60	9.166	2431	2434	2435	rBV3	997	487	0.03%	0.003%
61	9.208	2443	2447	2448	rBV4	780	473	0.02%	0.003%
62	9.250	2457	2460	2463	rBV5	1177	869	0.05%	0.006%
63	9.269	2463	2466	2467	rBV3	1078	517	0.03%	0.003%
64	9.420	2500	2513	2537	rBV	723317	1286892	66.96%	8.145%
65	9.671	2588	2591	2594	rBV4	1382	1093	0.06%	0.007%
66	9.861	2647	2650	2651	rBV2	1347	625	0.03%	0.004%
67	9.903	2660	2663	2667	rBV5	1466	1388	0.07%	0.009%
68	10.208	2754	2758	2759	rBV5	1086	770	0.04%	0.005%
69	10.340	2796	2799	2800	rBV3	1197	662	0.03%	0.004%
70	10.411	2818	2821	2825	rBV6	1121	717	0.04%	0.005%
71	10.472	2838	2840	2841	rBV2	754	260	0.01%	0.002%
72	10.710	2912	2914	2916	rBV3	1015	467	0.02%	0.003%
73	10.758	2917	2929	2949	rVB	622204	1021931	53.17%	6.468%
74	11.070	3024	3026	3028	rBV3	798	334	0.02%	0.002%
75	11.086	3029	3031	3034	rVV3	916	595	0.03%	0.004%
76	11.202	3063	3067	3070	rBV6	1124	734	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
 Data File : VU047100.D
 Acq On : 11 Feb 2022 01:32
 Operator : SY/MD
 Sample : N1462-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

77	11.256	3082	3084	3088	rBV6	663	470	0.02%	0.003%
78	11.275	3088	3090	3092	rBV3	915	555	0.03%	0.004%
79	11.629	3195	3200	3207	rBV9	1739	2542	0.13%	0.016%
80	11.697	3213	3221	3227	rBV10	3864	6125	0.32%	0.039%
81	11.812	3244	3257	3279	rBV	818595	1315063	68.42%	8.323%
82	12.192	3360	3375	3392	rBV	901584	1472900	76.63%	9.322%
83	12.500	3469	3471	3473	rBV3	1299	619	0.03%	0.004%
84	13.134	3664	3668	3671	rBV4	1397	1395	0.07%	0.009%
85	13.218	3691	3694	3700	rBV7	1596	1488	0.08%	0.009%
86	13.330	3727	3729	3732	rBV3	1086	485	0.03%	0.003%
87	13.369	3737	3741	3743	rBV5	1031	854	0.04%	0.005%
88	13.446	3763	3765	3767	rBV2	1222	641	0.03%	0.004%
89	13.738	3854	3856	3860	rVB5	752	568	0.03%	0.004%
90	13.761	3860	3863	3864	rBV3	868	500	0.03%	0.003%
91	13.838	3883	3887	3889	rBV4	1635	1451	0.08%	0.009%




Sum of corrected areas: 15799818

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
Data File : VU047100.D
Acq On : 11 Feb 2022 01:32
Operator : SY/MD
Sample : N1462-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

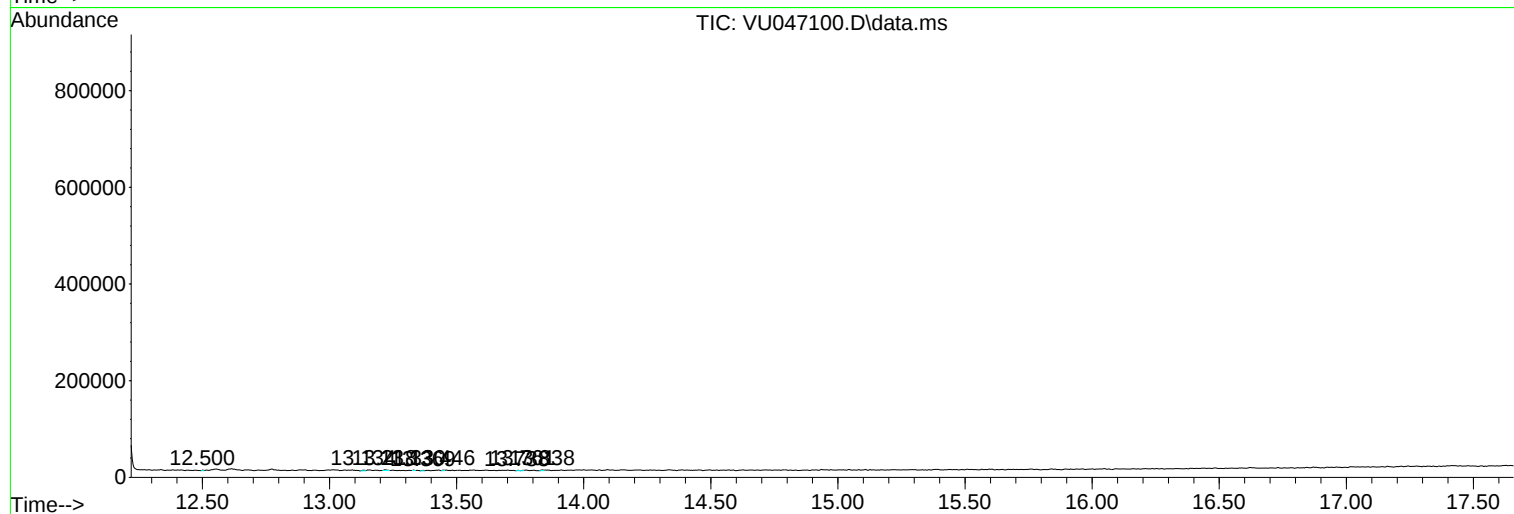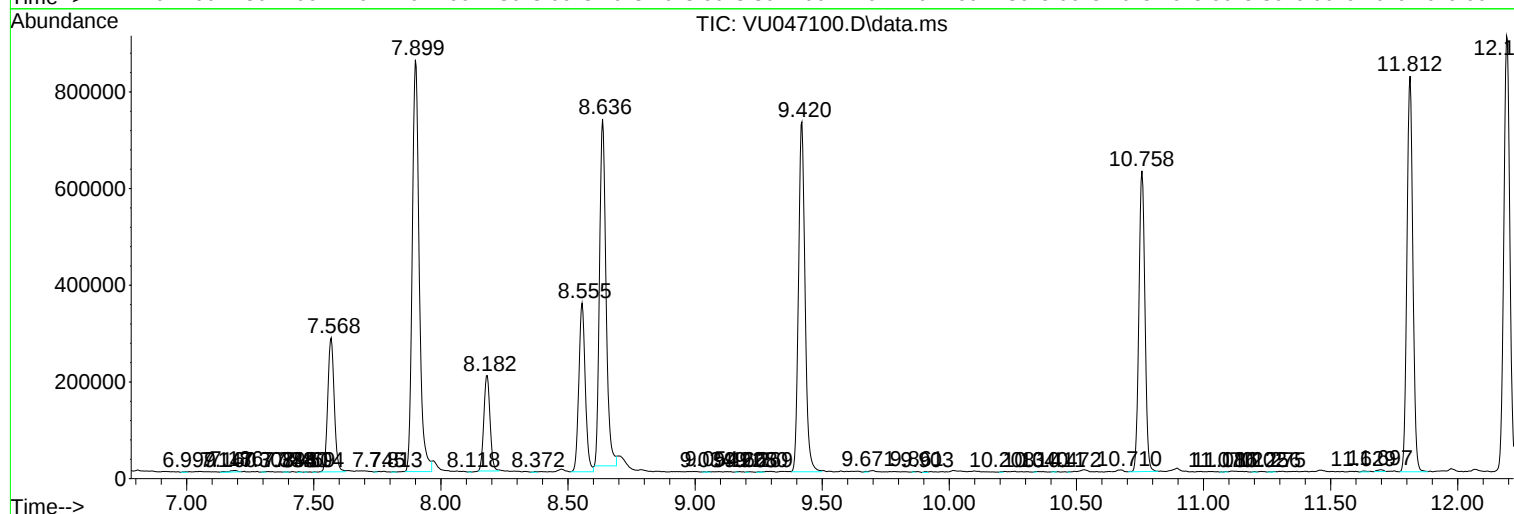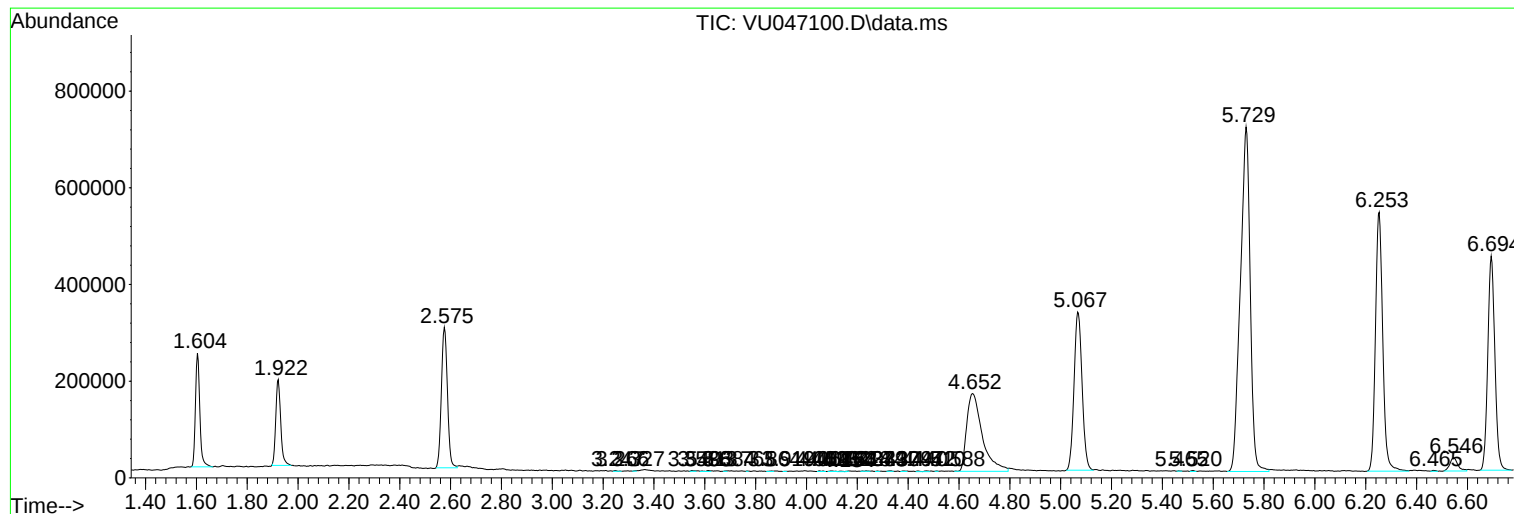

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
Data File : VU047100.D
Acq On : 11 Feb 2022 01:32
Operator : SY/MD
Sample : N1462-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021022\
Data File : VU047100.D
Acq On : 11 Feb 2022 01:32
Operator : SY/MD
Sample : N1462-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc