


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021025\
Data File : VU063218.D
Acq On : 10 Feb 2025 09:06
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Feb 11 08:42:19 2025

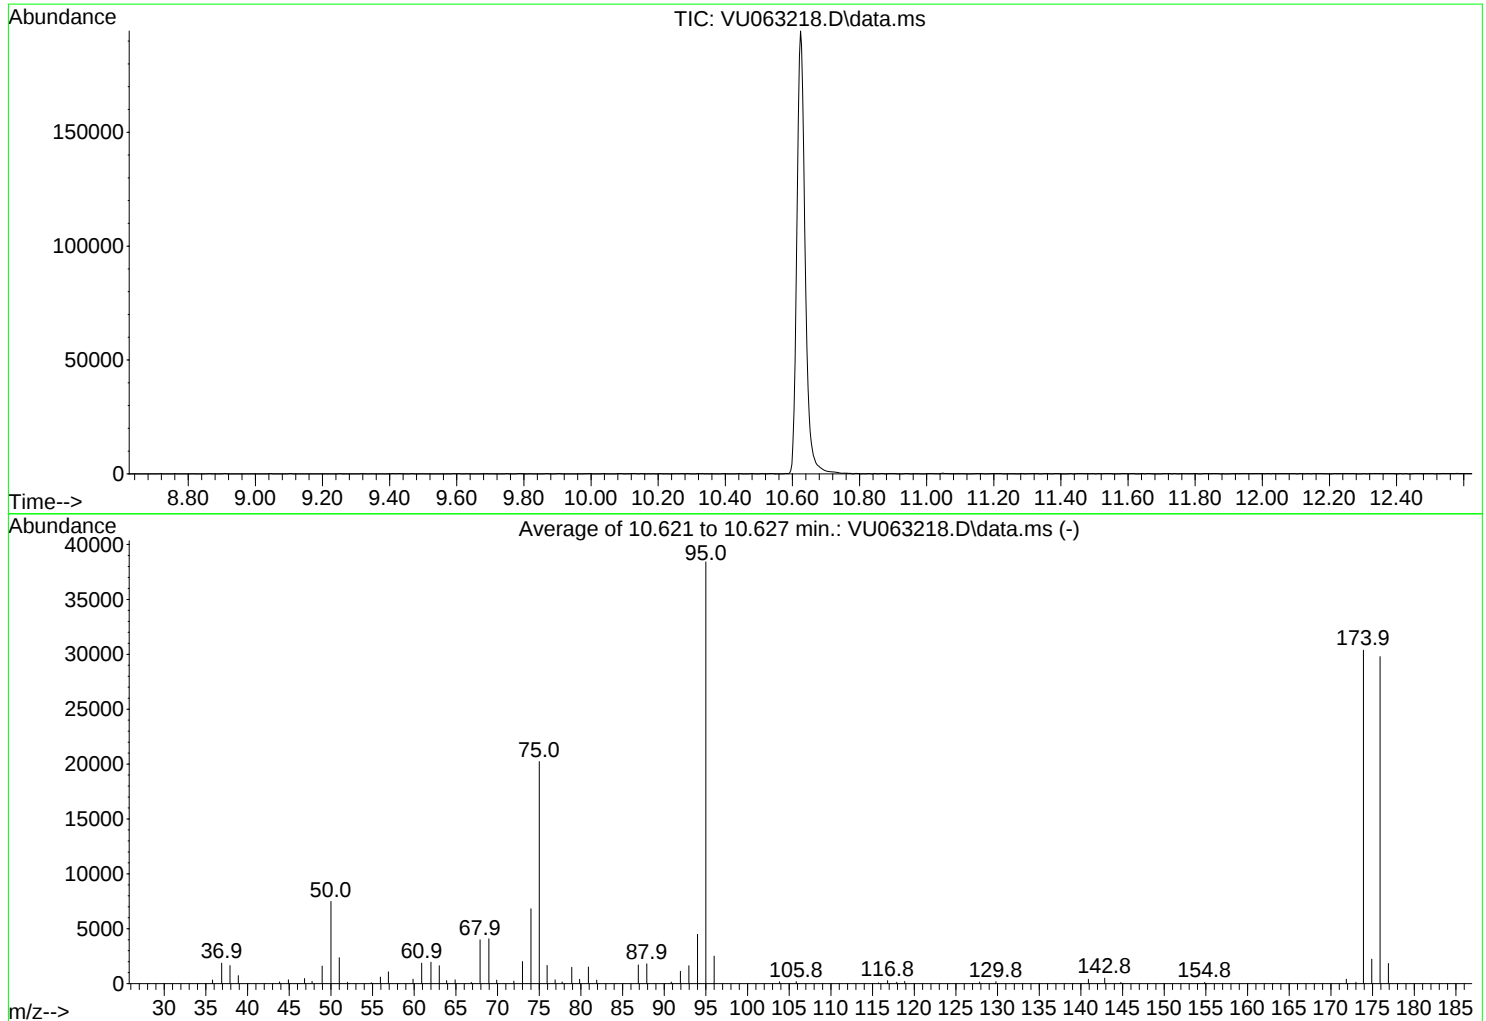

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.5	7489	PASS
75	95	30	60	52.7	20232	PASS
95	95	100	100	100.0	38421	PASS
96	95	5	9	6.5	2505	PASS
173	174	0.00	2	0.5	139	PASS
174	95	50	100	79.1	30381	PASS
175	174	5	9	7.3	2224	PASS
176	174	95	101	98.1	29792	PASS
177	176	5	9	6.2	1844	PASS